

Digital Oscilloscope & Multimeter

GDS-122

USER MANUAL

GW INSTEK PART NO.



ISO-9001 CERTIFIED MANUFACTURER

GW INSTEK

勝特力材料 886-3-5753170
勝特力电子(上海) 86-21-34970699
勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

October 2007 edition

This manual contains proprietary information, which is protected by copyrights. All rights are reserved. No part of this manual may be photocopied, reproduced or translated to another language without prior written consent of Good Will company.

The information in this manual was correct at the time of printing. However, Good Will continues to improve products and reserves the rights to change specification, equipment, and maintenance procedures at any time without notice.

Windows is a registered trademark of Microsoft Corporation in the United States and other countries.

Good Will Instrument Co., Ltd.

No. 7-1, Jhongsing Rd., Tucheng City, Taipei County 236, Taiwan.

TABLE OF CONTENTS

Safety Instructions	6
Getting Started	9
Package Contents	10
Main Features	11
Front Panel and Keys Overview	12
Manual Overview	14
Using the Oscilloscope	15
Basic Operations	16
1. Powering up the GDS-122	16
2. Connecting an input signal	17
3. Using the Autoset function	18
4. Introducing the display contents	19
5. Adjusting waveform scales	20
6. Adjusting waveform positions	21
Configurations	22
Configuring channel (vertical) settings	22
Configuring horizontal settings	25
Configuring trigger settings: general settings	27
Configuring trigger settings: edge triggering	30
Configuring trigger settings: video triggering	33
Selecting the acquisition mode	35
Configuring display settings	36
Viewing the system status	37
Measurements	39
Running waveform maths	39
Running automatic measurements	41
Running time cursor measurements	42
Running voltage cursor measurements	43
Advanced Viewings	45
Zooming waveforms horizontally	45

Viewing waveforms in X-Y format	47
Viewing signal peaks	48
Viewing noisy signals	49
Viewing variations in a signal	50
Calibration	51
Running the self calibration	51
Running the probe calibration	52
Saving/Recalling Waves and Settings	53
Recalling the default settings	53
Saving waveforms	54
Recalling waveforms	55
Menu Tree / Operation Shortcuts	56
Trigger	56
CH1/CH2 Setup	56
Measurement Setup 1/2	57
Wave Math	57
Cursor Measurement	57
Acquisition Mode	58
Time Mode	58
Function	58
Display	58
Wave Save	59
System Status	59
OSC OPTION key	60
Using the Software	61
Installing the software	62
Modifying/Reinstalling/Uninstalling the software	64
Activating the software and connecting the GDS-122 ..	65
Configuring the screen	68
Viewing the waveforms	71
Using the cursor measurements	75
Saving waveforms	77
Recalling waveforms	79
Printing out waveforms	80
Accessing the Help	82
Using the Multimeter	83
Activating the Multimeter	84

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Measuring Voltage	85
Measuring Current	87
Measuring Impedance	89
Measuring Diode	91
Measuring Continuity	92
Measuring Capacitance	93
Faq.....	95
Specifications.....	97
Oscilloscope specifications	97
Multimeter specifications	98
General specifications	99
Declaration of Conformity.....	100
Index.....	101







勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

SAFETY INSTRUCTIONS


This chapter contains important safety instructions that you should follow when operating the instrument and when keeping it in storage. Read the following before any operation to ensure your safety and to keep the instrument in best condition.

Safety Symbols

These symbols may appear in this manual or on the instrument.

	WARNING	Warning: Identifies conditions or practices that could result in injury or loss of life.
	CAUTION	Caution: Identifies conditions or practices that could result in damage to the instrument or to other properties.
		DANGER: High Voltage
		Attention: Refer to the Manual
		Protective Conductor Terminal
		Earth (ground) Terminal

Safety Guidelines

- | | | | |
|---|----------------|--------------------|---|
|  | CAUTION | General Guidelines | <ul style="list-style-type: none"> Do not place heavy objects on the instrument. Avoid severe impacts or rough handlings that may damage the instrument. Avoid discharges of static electricity onto or near the instrument. Do not insert bare wires or metal objects into the terminals. Do not apply input voltage more than 42V peak (30Vrms) to the instrument. |
|---|----------------|--------------------|---|

- Do not perform measurements at a power generating source or building installation site (see note below).
- The instrument should only be disassembled by a qualified technician.

(Measurement categories) EN 61010-1:2001 specifies the measurement categories and their requirements as follows. This instrument falls under category I. Measurement category IV is for measurement performed at the source of low-voltage installation. Measurement category III is for measurement performed in the building installation. Measurement category II is for measurement performed on the circuits directly connected to the low voltage installation. Measurement category I is for measurements performed on circuits not directly connected to Mains.

Power Supply



WARNING

- AC Input voltage: 100 to 240V, 50/60Hz
- The power supply voltage should not fluctuate more than 10%.
- Always use the AC adaptor included in the package.
- Always connect the AC adaptor to the mains line first, then to the instrument.

Cleaning the instrument

- Disconnect the power cord before cleaning the instrument.
- Use a soft cloth dampened in a solution of mild detergent and water. Do not spray liquid into the instrument.
- Do not use chemicals or cleaners containing harsh products such as benzene, toluene, xylene, and acetone.

Operation Environment

- Location: Indoor, no direct sunlight, dust free, most non-conductive pollution (see note below)
- Relative Humidity: < 75%
- Altitude: < 2000m
- Temperature: 0°C to 40°C

(Pollution Degree) EN 61010-1:2001 specifies the pollution degrees and their requirements as follows. This instrument falls under degree 2. Pollution refers to "addition of foreign matter, solid, liquid, or gaseous (ionized gases), that may produce a reduction of dielectric strength or surface resistivity".

Pollution degree 1: No pollution or only dry, non-conductive pollution occurs. The pollution has no influence.

Pollution degree 2: Normally only non-conductive pollution occurs.

Occasionally, however, a temporary conductivity caused by condensation must be expected.

Pollution degree 3: Conductive pollution occurs, or dry, non-conductive pollution occurs which becomes conductive due to condensation which is expected. In such conditions, equipment is normally protected against exposure to direct sunlight, precipitation, and full wind pressure, but neither temperature nor humidity is controlled.

Storage environment

- Location: Indoor
- Relative Humidity: < 75%
- Temperature: -10°C to 70°C

Power cord for the United Kingdom

When using the instrument in the United Kingdom, make sure the power cord meets the following safety instructions.

NOTE: This lead/appliance must only be wired by competent persons

WARNING: THIS APPLIANCE MUST BE EARTHED

IMPORTANT: The wires in this lead are coloured in accordance with the following code:

Green/ Yellow:	Earth
Blue:	Neutral
Brown:	Live (Phase)



As the colours of the wires in main leads may not correspond with the colours marking identified in your plug/appliance, proceed as follows:

The wire which is coloured Green & Yellow must be connected to the Earth terminal marked with the letter E or by the earth symbol or coloured Green or Green & Yellow.

The wire which is coloured Blue must be connected to the terminal which is marked with the letter N or coloured Blue or Black.

The wire which is coloured Brown must be connected to the terminal marked with the letter L or P or coloured Brown or Red.

If in doubt, consult the instructions provided with the equipment or contact the supplier.

This cable/appliance should be protected by a suitably rated and approved HBC mains fuse: refer to the rating information on the equipment and/or user instructions for details. As a guide, cable of 0.75mm² should be protected by a 3A or 5A fuse. Larger conductors would normally require 13A types, depending on the connection method used.

Any moulded mains connector that requires removal /replacement must be destroyed by removal of any fuse & fuse carrier and disposed of immediately, as a plug with bared wires is hazardous if engaged in live socket. Any re-wiring must be carried out in accordance with the information detailed on this label.

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

GETTING STARTED










This chapter gives you an overview of what the GDS-122 is about, what items are included in the package, and how the user manual is organized. After opening the GDS-122 package, check the contents referring to the *Package Contents* section, then learn the features and interface reading the *Main Features* and *Front Panel and Keys Overview* section. The *Manual Overview* section gives you an overall picture of what each chapter is about, helping you directly jump to the relevant location.



Package Contents	10
Main Features	11
Front Panel and Keys Overview	12
Manual Overview	14

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Package Contents


Soft carrying case 	GDS-122 
AC-DC adaptor 	Oscilloscope probe x 2 + probe adjustment tools 
1kHz square wave output cable 	Multimeter test lead x 2 
Extension module for large current measurement 	Extension module for small capacitance measurement 
USB communication cable 	CD-ROM (software)
User Manual (this document)	RS-232C communication cable (optional item - contact Good Will)

Main Features

Oscilloscope	<ul style="list-style-type: none"> Dual channel 20MHz bandwidth 100MS/s real-time sampling rate $\leq 17.5\text{ns}$ rising time 5ns to 5s/div horizontal scale 5mV to 5V/div vertical scale 6k memory points per channel Isolated inputs between oscilloscope and multimeter Autoset function Trigger mode: Auto, Free run, Single shot, Edge, Video 2 cursors 5 automatic measurements 4 display image memories Auto-calibration
Multimeter	<ul style="list-style-type: none"> Volts, Amps, Ohms, Continuity, Diode, Capacitance measurement 20A maximum amplitude True RMS measurement Isolated inputs between oscilloscope and multimeter
Common	<ul style="list-style-type: none"> USB interface RS-232C interface 1kHz square wave output 3.8 inch color LCD display, 320 x 240 resolution 6 hours running time Li-ion battery 180mm x 113mm x 40mm compact size 690g light weight

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Front Panel and Keys Overview

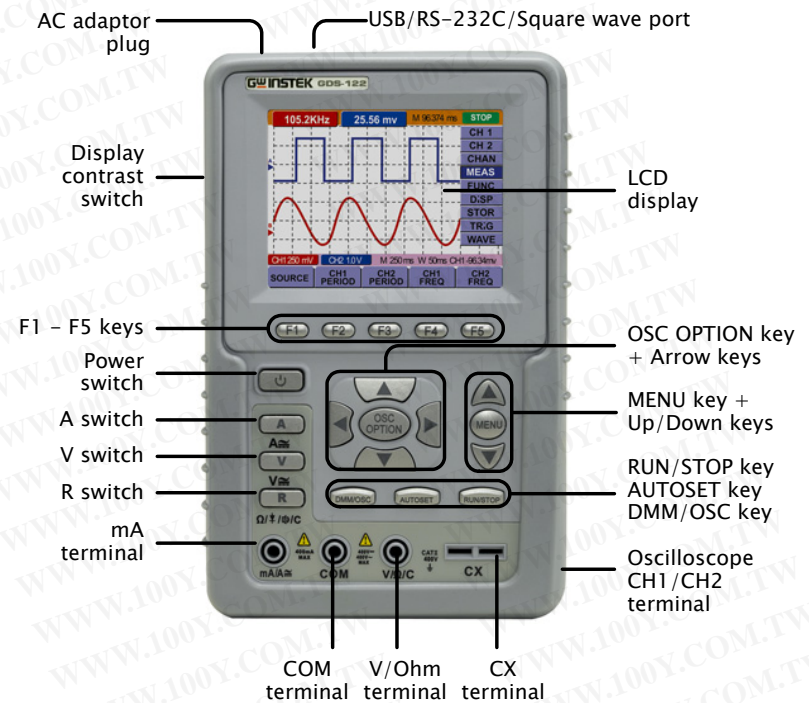

DSO : Oscilloscope function **DMM** : Multimeter function

AC adaptor plug	Accepts the AC adaptor cord. DC 8.5V, 1500mA.
USB port	Accepts the USB cable for PC connection.
RS-232C port	Accepts the optional RS-232C cable for PC connection.
Square wave output	Outputs a 1kHz square wave for probe compensation and other general purposes.
LCD display	3.8 inch, 320 x 240 resolution, color LCD display.
OSC OPTION key + Arrow keys	DSO Sets the following parameters: vertical level and scale (page22), horizontal level and scale (page25), trigger level (page25), and cursor position (page42).

MENU key + Up/Down keys	DSO	Activates the side menu and selects the menu items.
RUN/STOP key	DSO	Manually turns on (run) or off (stop) the trigger. For details, see page25.
RUN/STOP key	DMM	Freezes (stop) or unfreezes (run) the measurement.
AUTOSET key	DSO	Automatically selects the horizontal scale, vertical scale, and trigger level according to the input signal. See page18 for details.
	DMM	Switches the measurement mode. For details, see page87(current), page85(voltage), and page89(impedance).
DMM/OSC key		Switches the operation mode between the oscilloscope and multimeter.
CH1 / 2 terminal	DSO	Accepts the CH1 and CH2 input signal.
CX terminal	DMM	Accepts the test leads for capacitor measurement.
V/Ω terminal	DMM	Accepts the red lead for voltage, small capacitance, and impedance measurements.
COM terminal	DMM	Accepts the black (ground) lead.
mA terminal	DMM	Accepts the red lead for current measurement.
R switch	DMM	Selects the following measurement: impedance (page89), diode (page91), continuity (page92), capacitance (page93).
V switch	DMM	Selects voltage measurements (page85).
A switch	DMM	Selects current measurements (page87).
Power switch		Turns on or off the GDS-122 power.
F1 – F5 keys		Selects the menu item at the bottom of the display.
Disp contrast sw		Selects the display contrast.

Manual Overview

Overview	This user manual is comprised of seven chapters. If you want to jump start using the GDS-122, go directly to the <i>Using Oscilloscope</i> or <i>Using Multimeter</i> chapter.
Safety Instructions (page6)	The <i>Safety Instructions</i> gives you an overview of important safety-related issues which you should be aware of before, during, and after operations.
Getting Started (page9)	The <i>Getting Started</i> chapter provides you with the overview of the GDS-122: main features, package contents, front panel, and user manual (this section).
Using the Oscilloscope (page15)	The <i>Using the Oscilloscope</i> chapter describes in detail how to use the GDS-122's oscilloscope functionalities, including the PC software. The chapter starts with simple, basic operations toward more complex measurements and settings. If you are new to the GDS-122, start with the Basic Operations section. For advanced users, the <i>Menu Tree / Shortcuts</i> section shows the menu structures and all operations shortcuts.
Using the Multimeter (page83)	The <i>Using the Multimeter</i> chapter describes how to use the GDS-122's multimeter functionalities. The most commonly used Voltage, Current, and Resistance sections are listed in the front.
Faq (page95)	The <i>Faq</i> chapter lists major problems you might encounter during operations and how to fix or avoid them. Most issues are also listed in the relevant chapters throughout the document.
Specifications (page97)	The GDS-122 specifications are separated in oscilloscope, multimeter, and general parts.
Declaration of conformity (page100)	The <i>Declaration of Conformity</i> chapter lists the safety and EMI/EMC standards to which the GDS-122 conforms.
Index (page101)	The <i>Index</i> chapter lists most of the keywords used in this manual in an alphabetical order.

USING THE OSCILLOSCOPE

This chapter describes the oscilloscope functionalities in the GDS-122: setting it up and measuring simple waveforms, using advanced measurement functions, and configuring the system settings. The menu tree section at the end gives you an overview of all functionalities and a quick access to each of them. For the multimeter functionalities, see page83.

Basic Operations.....	16
Configurations	22
Measurements	39
Advanced Viewings	45
Calibration	51
Saving/Recalling Waves and Settings	53
Menu Tree / Operation Shortcuts	56
Using the Software.....	61

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Basic Operations

- Operation flow** The *Basic Operations* section describes how to set up the GDS-122 and observe an input signal, step-by-step.
1. Powering up the GDS-122
 2. Connecting an input signal
 3. Using the Autoset / Introducing the display
 4. Adjusting the scales
 5. Adjusting the waveform position

- Advanced operations** For more advanced or detailed operations, see the following chapters.
- *Configurations* (page22)
 - *Measurements* (page39)
 - *Advanced Viewings* (page45)
 - *Calibrations* (page51)

1. Powering up the GDS-122

- 1. Pressing the power switch** Press the power switch. The welcome screen with the corporate logo appears on the display.



To adjust the display brightness, press the switch on the side. The backlight turns on and off.



- 2. Activating the oscilloscope** Press any key (for example the MENU (Example) key) to enter the oscilloscope mode. See the battery level icon at the top left corner of the display and connect the



power cord if the level is < 25%.



Switching the operation mode

If the multimeter screen appears, press the DMM/OSC key and change the mode to oscilloscope.



Tilt standing the GDS-122

Use the bar at the back to tilt stand the GDS-122 on a horizontal plane.



Note


If pressing the power switch does not turn on the GDS-122, the battery may need recharging. Connect the GDS-122 to the AC adaptor and recharge it for at least 15 minutes.

2. Connecting an input signal

1. Connecting the probe


Connect the probe(s) between the DUT (Device Under Test) and the CH1/2 inputs on the GDS-122.

Alternately, you may use the GDS-122's own 1kHz square wave output signal. Insert the signal cable (included in the package) to the output terminal.




2. Setting the probe attenuation

To prevent excessive input voltage, we recommend you to set the probe attenuation level to the X 10 position to prevent excessive voltage.

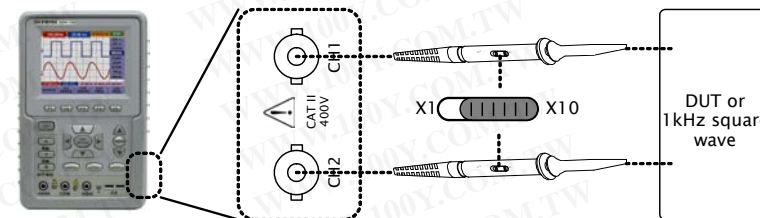

3. Setting the display magnification

1. After attenuating the probe level by x10, you also need to magnify the display level by x10 to match the displayed amplitude with the real amplitude. Open the CH1 or CH2 SETUP menu by pressing the MENU key and using the Up/Down keys.
2. Select the probe attenuation level (10X) by pressing F3 (Probe) repeatedly. The CH1/CH2 vertical scale indicator at the bottom left corner of the display changes accordingly.

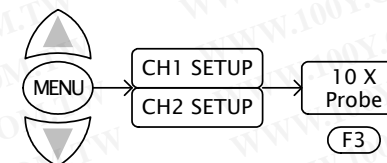

3. Using the Autoset function

Overview

The Autoset function automatically configures the following parameters according to the input signal.

- CH1/CH2 on/off
- Vertical scale/level
- Horizontal scale/level
- Trigger level


Using the Autoset function

Press the AUTOSET key. The input signal appears in the best display condition.




(Continued on next page)

Example

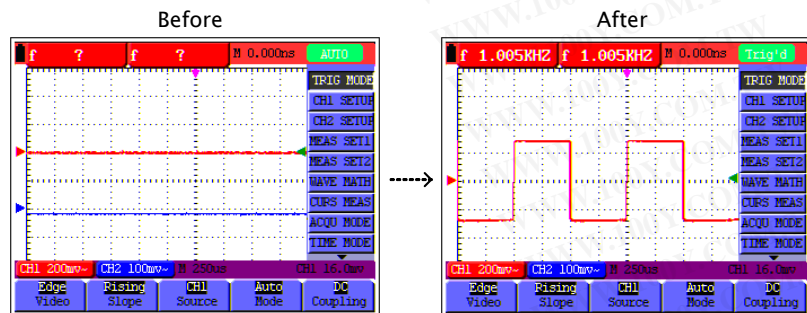

4. Introducing the display contents

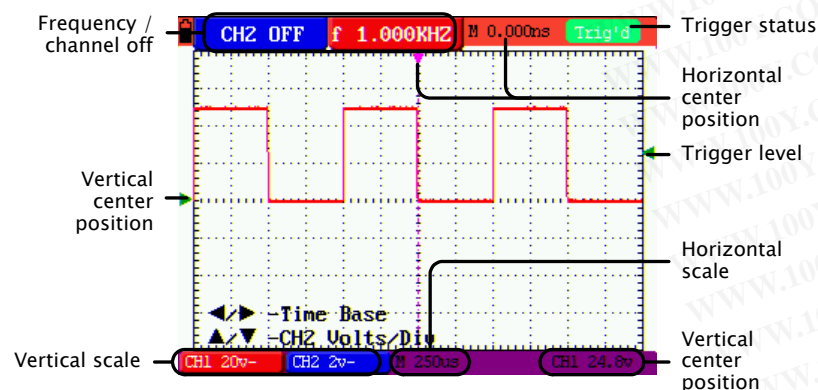


- Trigger status
- Updating the signal (auto mode) **AUTO**
 - The signal is triggered **Trig'd**
 - Waiting for trigger conditions **Ready**
 - Triggering is stopped **STOP**

Press the RUN/STOP key to control trigger on/off (run/stop). **RUN/STOP**

5. Adjusting waveform scales

Selecting the menu

Press the OSC OPTION key repeatedly until the following menu appears on the display.



◀/▶ – Time Base

▲/▼ – CH1 (or CH2) Volts/Div




Vertical scale

Horizontal scale


Adjusting the horizontal scale

Use the Left/Right key to change the horizontal scale.

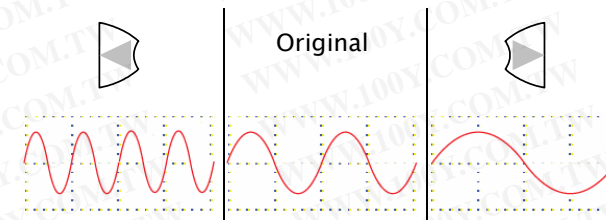

Adjusting the vertical scale

Use the Up/Down key to change the vertical scale.

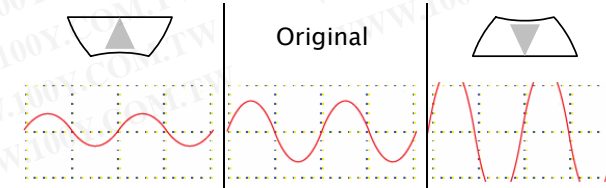

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)



6. Adjusting waveform positions

Selecting the menu

Press the OSC OPTION key repeatedly until the following menu appears on the display.


◀/▶ – Time

▲/▼ – CH1 (or CH2) Zero

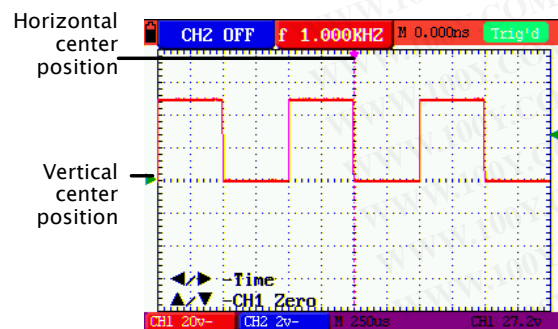


Adjusting the horizontal position

Use the Left/Right key to change the horizontal position.

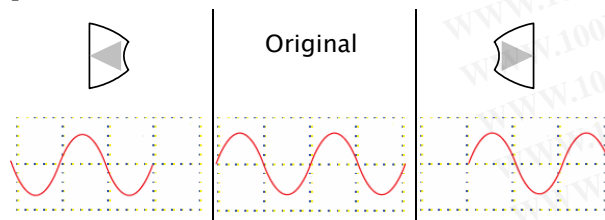

Adjusting the vertical position

Use the Up/Down key to change the vertical position.

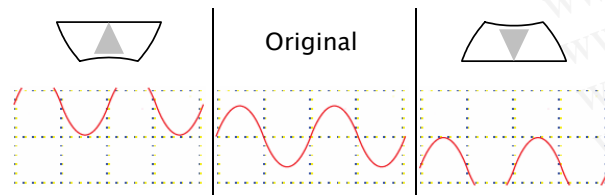

Configurations

Overview

The configuration chapter describes how to change various GDS-122 internal parameters for allowing better measurement condition.

Configuration items

- Channel (vertical) settings page22
- Horizontal settings page25
- Trigger settings page25
- Acquisition modes page30
- Display settings page36
- System status (only for viewing) page37

Configuring channel (vertical) settings

Overview

The channel settings configure how the waveform appears in terms of vertical or voltage scale.

Position Sets the vertical position of the waveform.

Scale Sets the vertical scale (volts per graticule). Range: 5mV/div to 5V/div

CH on/off Turns the channel on or off.


Coupling Selects AC or DC coupling. The DC coupling shows all signal elements, while the AC coupling filters out the DC component from the waveform.

Inversion Flips the waveform upside down.


Magnification Magnifies the displayed units (does not magnify the real signal). The magnification function is useful to align the displayed with probe attenuation (page17), especially X10.

Setting the vertical position

1. Press the OSC OPTION key repeatedly until the following menu appears on the display.
 ◀/▶ – Time
 ▲/▼ – CH1 (or CH2) Zero




2. Use the Up/Down key to change the vertical position.

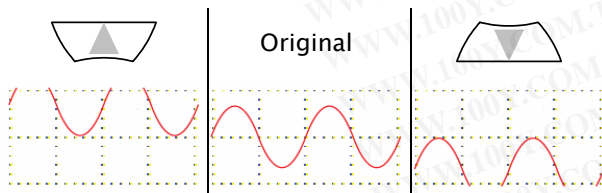


Setting the vertical scale

1. Press the OSC OPTION key repeatedly until the following menu appears on the display.
 ◀/▶ – Time Base
 ▲/▼ – CH1 (or 2) Volts/Div




2. Use the Up/Down key to change the vertical scale.

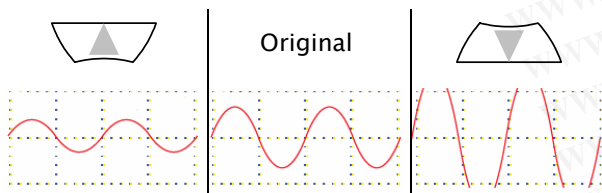

Turning the channel on/off

1. Press the MENU key and use the Up/Down keys to select the CH1(CH2) SETUP menu.
2. Press F2 (Channel) repeatedly to turn on or off the channel.


勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

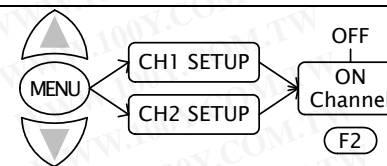

Note that when using the Autoset function (page18), channels are automatically turned on or off.

Selecting the coupling mode

1. Press the MENU key and use the Up/Down keys to select the CH1(CH2) SETUP menu.
2. Press F1 (Coupling) repeatedly to select DC, AC, or Ground coupling.

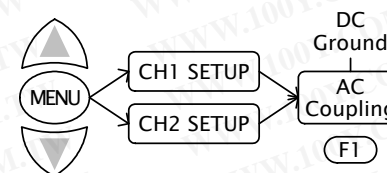


The DC coupling shows both DC and AC signal.

The AC coupling only shows the AC signal.

The Ground coupling shows the ground line.

DC coupling

(center point is at the bottom due to DC offset)

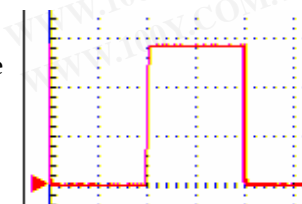



AC coupling

(center point is at the middle since the DC offset is being removed)




Inverting the channel

1. Press the MENU key and use the Up/Down keys to select the CH1(CH2) SETUP menu.
2. Press F4 (Inverted) to invert the waveform.

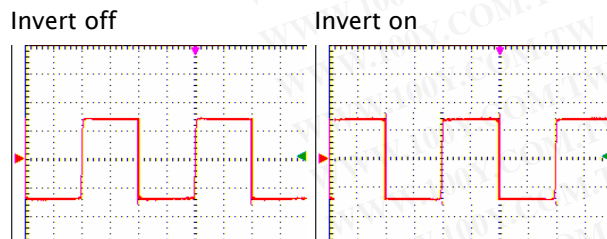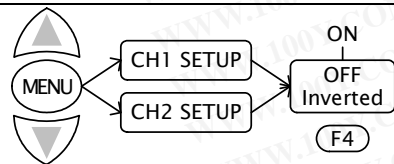

Selecting the magnification

1. Press the MENU key and use the Up/Down keys to select the CH1(CH2) SETUP menu.
2. Press F3 (Probe) repeatedly to select the probe magnification ratio.

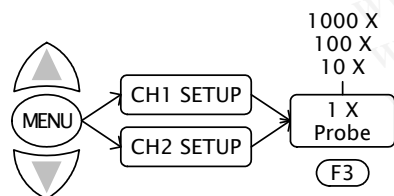

Configuring horizontal settings

Overview


The horizontal settings configure how the waveform appears in terms of horizontal or time scale.

Position Sets the horizontal position of the waveform.


Scale Sets the horizontal scale (time per graticule). Range: 100ms/s to 10s/s

Setting the horizontal position

1. Press the OSC OPTION key repeatedly until the following menu appears on the display.
◀/▶ – Time



2. Use the Left/Right key to change the horizontal position.

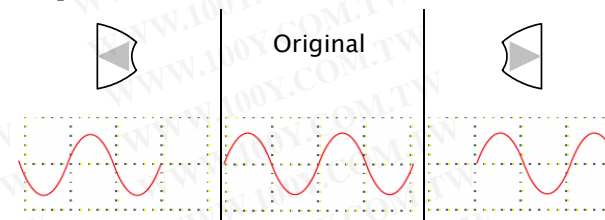


Selecting the horizontal scale

1. Press the OSC OPTION key repeatedly until the following menu appears on the display.

◀/▶ – Time Base



2. Use the Left/Right key to change the horizontal scale.

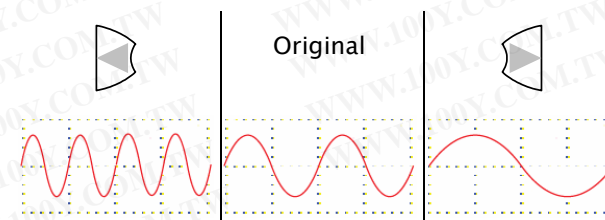

Configuring trigger settings: general settings

Overview

The trigger settings configure how the incoming signal is triggered. The general settings section describes how to start and stop triggering, adjust the level, and change the trigger mode.

- For edge triggering details, see page30.
- For video triggering details, see page33.

Status Shows the triggering status in the icon appearing in the upper right corner of the display.

Run/Stop Controls starting and stopping the trigger.


Level Adjusts the vertical and horizontal level on which the waveforms are triggered.

Trigger status The trigger status icon is located at the top right corner of the display.

- Trig'd** The trigger condition is met.
- AUTO** The GDS-122 is showing the input signal waveform regardless of trigger condition. Available in the Auto trigger mode in edge triggering (page30).
- Ready** The trigger condition is not met, and the GDS-122 is waiting for the next condition. Available in the Normal trigger mode in edge triggering (page30).
- Scan** The GDS-122 is showing the input signal waveform regardless of trigger condition. The waveform is gradually updated from the left side of the display. The GDS-122 automatically switches to the Scan when the horizontal scale is at 100ms/div or longer.
- STOP** Triggering is stopped regardless of the trigger condition. In order to restart

triggering, you have to press the RUN/STOP key again (in single trigger mode) or switch to another trigger mode.

Horizontal scale vs. trigger status

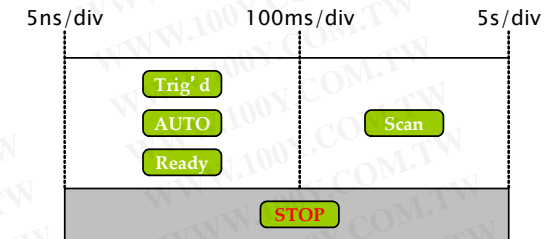

Run/Stop

Pressing the Run/Stop key once stops triggering at most situations and changes the trigger icon to STOP.



In the single trigger mode in edge triggering (page30), pressing the RUN/STOP key works as both activating and deactivating trigger.

Trigger level

Press the OSC OPTION key repeatedly until the following menu appears on the display.




◀/▶ – Time
▲/▼ – Trig




Trigger level indicators

Trigger level (horizontal)

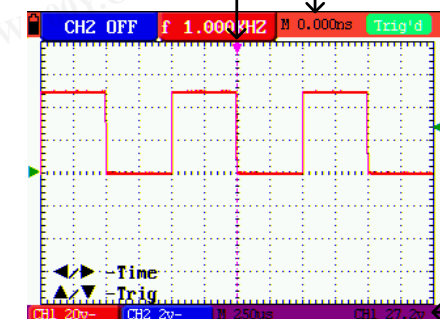


Trigger level (vertical)


Use the arrow keys to change the triggering position.

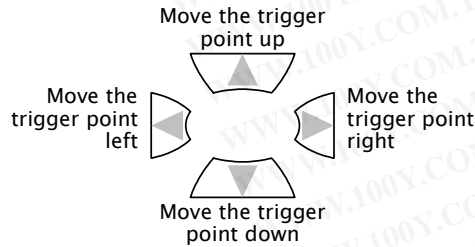

Pressing the Up and Down key together resets the vertical trigger level to zero.



Pressing the Left and Right key together resets the horizontal trigger level to zero.



Configuring trigger settings: edge triggering


Overview

The edge trigger type triggers on the incoming signal edge. Use the edge trigger for all signals except for video related ones.

- For general trigger settings, see page27.
- For video triggering details, see page33.


To select edge triggering, follow these steps.

1. Press the MENU key and use the Up/Down keys to select TRIG MODE menu.
2. Press F1 (Type) to select the Edge trigger type.

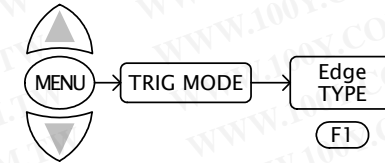


Slope	Selects the slope, rising or falling, on which the GDS-122 triggers the input signals.
Source	Selects the signal source channel, CH1 or CH2.
Mode	Selects the triggering mode, Auto (acquires signal continuously), Normal (acquires signal when trigger conditions are met), and Single (manually triggers the signal).
Coupling	Selects the DC or AC coupling and rejection filters: high frequency or low frequency.

Selecting the trigger slope Press F2 (Slope) repeatedly to select the rising or falling slope.





(Continues to the next page)

Example: falling edge

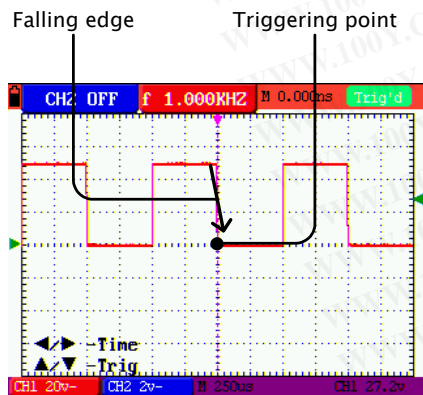


Selecting the source channel

Press F3 (Channel) repeatedly to select the trigger source channel, CH1 or CH2. The trigger channel indicator at the bottom right corner of the display changes.



Selecting the trigger mode

Press F4 (Mode) repeatedly to select the trigger mode. The trigger status icon in the upper right corner of the display changes accordingly. For the overview of trigger status in general, see page 27.



Auto mode

In the auto mode, input signals are constantly acquired and shown in the display regardless of trigger condition.

Horizontal scale (/div)	5ns	100ms	5s
Status icon when triggered	Trig'd	Scan	
Status icon when not triggered	AUTO	Scan	

Normal mode

In the normal mode, input signals are shown in the display only if the trigger condition is met.

Horizontal scale (/div)	5ns	100ms	5s
Status icon when triggered	Trig'd	Scan	
Status icon when not triggered	Ready	Scan	

Single mode


In the single mode, you manually trigger the GDS-122 by pressing the RUN/STOP key each time you need to observe the waveform. Once the waveform is captured, the GDS-122 stops triggering and waits for the next trigger command.

Horizontal scale (/div)	5ns	100ms	5s
Status icon when triggered	STOP	STOP	
Status icon when not triggered	AUTO ↕ Ready	Scan	

Selecting the coupling mode

Press F5 (Coupling) repeatedly to select the trigger coupling.

- AC: triggers only on the AC portion of the waveform.
- DC: triggers on the whole waveform (AC + DC).
- LF Rjc: filters out the lower frequency when triggering.
- HF Rjc: filters out the higher frequency when triggering.



Configuring trigger settings: video triggering


Overview

The video trigger type is designed to capture the video signal format, NTSC, PAL, or SECAM. For any other signal type, use the edge trigger.

- For general trigger settings, see page27.
- For edge triggering details, see page30.

To select edge triggering, follow these steps.

- Press the MENU key and use the Up/Down keys to select TRIG MODE menu.
- Press F1 (Type) to select the video trigger type.

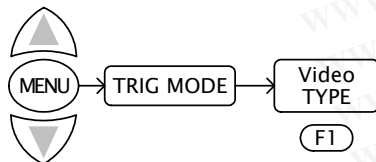


Polarity Selects the polarity of synchronization signal. Normal means the black level is low. Invert means the black level is high.

Source Selects the signal source channel, CH1 or CH2.

Sync Selects the part of the video signal used for synchronization: line or field.

Selecting the trigger polarity Press F2 (Polarity) repeatedly to select the polarity of synchronization signal.



- Normal: the black level is low.
- Inverted: the black level is high.



(Continues to the next page)

Selecting the source channel


Press F3 (Channel) repeatedly to select the trigger source channel, CH1 or CH2. The trigger channel indicator at the bottom right corner of the display changes.



Selecting the sync


Press F4 (Polarity) repeatedly to select the synchronization point.

- Line: the video line is used for triggering.
- Field: the video field is used for triggering.




Example

Video line trigger

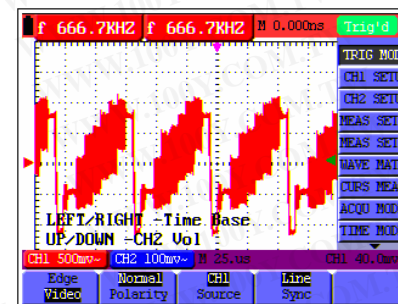


Video field trigger

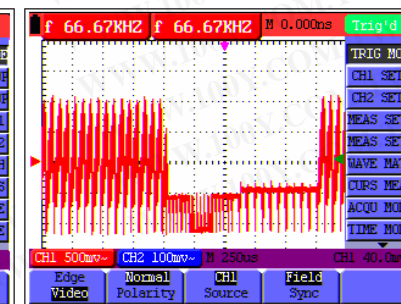


Selecting the acquisition mode

Overview	The acquisition mode specifies how the incoming analog signal is digitally sampled by the GDS-122.
Sample	The waveform data is sampled at an equal time interval. The sample mode accurately reconstructs the waveform, but cannot respond to rapid changes and sudden peaks.
Peak detect	The maximum and minimum data in the sampling interval are picked up. The peak detect mode captures rapid changes and sudden peaks, but the waveform becomes noisy.
Average	Multiple samples are averaged together. The average mode reduces the noise level, but the waveform must be repetitive. The number of averaging are 4, 16, 64, and 128.


Panel operations 1. Press the MENU key and select the ACQU MODE menu using the Up/Down keys.



2. Select the acquisition mode from F1 (Sample) to F3 (Average).




For the Average mode, also press F4 (Averages) repeatedly to select the number of averaging: 4, 16, 64, or 128.



Example


Sample Peak detect Average (16)

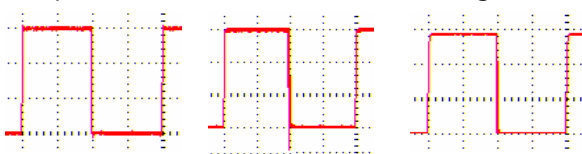


Configuring display settings

Overview	The display settings configure how the waveforms are drawn in the display.
vector drawing	The vector drawing mode shows the waveform as a smooth line, connecting each data point.
dot drawing	The dot drawing mode shows the waveform as a collection of independent data points.
persistence	The persistence setting sets how long the old waveforms remain in the display, useful for observing the waveform variations.


Panel operations 1. Press the MENU key and use the Up/Down keys to select the DISP SET menu.
2. Press F1 (Type) or F2 (Persist) repeatedly to select vector drawing, dot drawing, and persistence time.

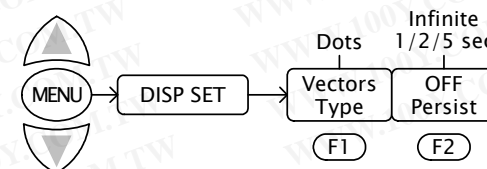

Vector/dot drawing example

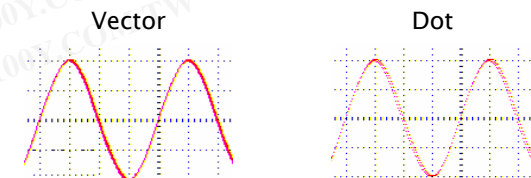




Persistence example

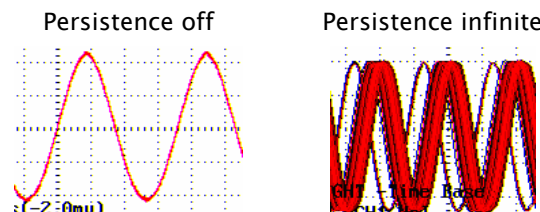

勝特力材料 886-3-5753170
勝特力电子(上海) 86-21-34970699
勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Viewing the system status

Overview The system status menu shows the GDS-122 system settings.

- Panel operations**
- Press the MENU key and select the SYS STAT menu using the Up/Down keys.
 
 - Select the status menu from F1 (Horizontal) to F4 (Misc) and press it. The status information appears in the display.
 
 - To close the system status screen, select different menus using the MENU key followed by Up/Down keys.
 

Horizontal status (F1)

HORIZONTAL SYSTEM STATUS	
TIME BASE	MAIN TIME BASE
MAIN SCALE	1.0ms
WINDOW SCALE	10.us
MAIN POSITION	300.0us
WINDOW POSITION	559.60us
DISPLAY FORMAT	YT
ACQUIRE MODE	SAMPLE

For details of each item, see the following pages.

Time base: page25

Main/window scale: page45

Main/window position: page45

Display format: page47 (XY)

Acquire mode: page35

(Continues to the next page)

Vertical status (F2)

VERTICAL SYSTEM STATUS		
SCALE	CH1	2.00v
SCALE	CH2	50.0mv
POSITION	CH1	0.00 divs(0.0mv)
POSITION	CH2	0.00 divs(0.0mv)
COUPLING	CH1	DC
COUPLING	CH2	DC
PROBE	CH1	1X
PROBE	CH2	1X
MATH	CH1-CH2	
INVERTED	CH1	OFF
INVERTED	CH2	OFF

For details of each item, see the following pages.

CH1/CH2 scale: page22

CH1/CH2 position: page22

CH1/CH2 coupling: page22

CH1/CH2 probe: page22

Math mode: page39

CH1/CH2 invert: page22

Trigger status (F3): Edge trigger

TRIGGER SYSTEM STATUS	
TYPE	EDGE
SOURCE	CH1
SLOPE	RISING
TRIGMODE	SINGLE TRIGGER
COUPLING	DC

For details of each item, see the following pages.

Trigger type: page30

Trigger source: page30

Trigger slope: page30

Trigger mode: page30

Trigger coupling: page30

Trigger status (F3): Video trigger

TRIGGER SYSTEM STATUS	
TYPE	VIDEO
SOURCE	CH1
POLARITY	NORMAL
SYNC	LINE

For details of each item, see the following pages.

Trigger type: page33

Trigger source: page33

Trigger polarity: page33

Trigger sync: page33

Misc status (F4)

MISC

Series Number
0739002
Ver 3.0

The Misc status shows the serial number and firmware version.

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Measurements

Overview The advanced measurement functions allow you to automatically measure various parameters in a waveform.

Measurement items	• Waveform math	page39
	• Automatic measurements	page41
	• Time cursor measurement	page42
	• Voltage cursor measurement	page43


Running waveform maths

Overview The waveform math function runs mathematical operations between CH1 and CH2 waveform, and then shows the result in the display.


Math type	• CH1 – CH2 (subtract CH2 from CH1)
	• CH2 – CH1 (subtract CH1 from CH2)
	• CH1 + CH2 (add CH1 and CH2)
	• CH1 * CH2 (multiply CH1 and CH2)
	• CH1 / CH2 (divide CH1 by CH2)

Panel operations 1. Make sure that both CH1 and CH2 waveforms are shown in the display.


2. Press the MENU key and select the WAVE MATH menu using the Up/Down keys.



3. Select the math operation from F1 (CH1 – CH2) to F5 (CH1 / CH2) and press it.



4. The math result appears in the display (example: adding two square waveforms)

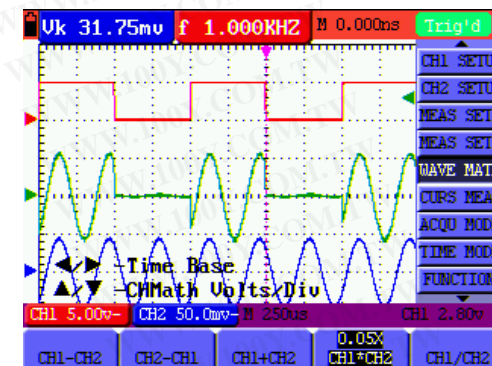

5. To cancel the math result, press the function key (F1 to F5) again.

Changing the math result position


1. Press the OSC OPTION key. Make sure the following menu appears on the display.



◀/▶ – Time
▲/▼ – CHM Zero



2. Use the arrow keys to move the math result position.



Changing the math result scale


1. Press the OSC OPTION key repeatedly until the following menu appears on the display.



◀/▶ – Time Base
▲/▼ – CHMath Volts/Div



2. Use the arrow keys to change the math result scale.



Saving or recalling the math result



The math result waveform can be saved into or recalled from one of the four GDS-122 internal memories. See page53 for details.

Running automatic measurements

Overview	The automatic measurement function measures the input signal's characteristics and lists them in the top left corner of the display.
Source signal	CH1, CH2
Measurement set	SET1, SET2
Measurement items	<p>The following measurement items are available.</p> <ul style="list-style-type: none"> • Frequency • Period • Mean voltage • Peak-to-peak voltage • Cycle voltage (true RMS)


Panel operations 1. Make sure that the waveform appears.

2. Press the MENU key and select the MEAS SET1 or SET2 menu using the Up/Down keys. SET1 and SET2 correspond to the results in the upper left corner of the display.

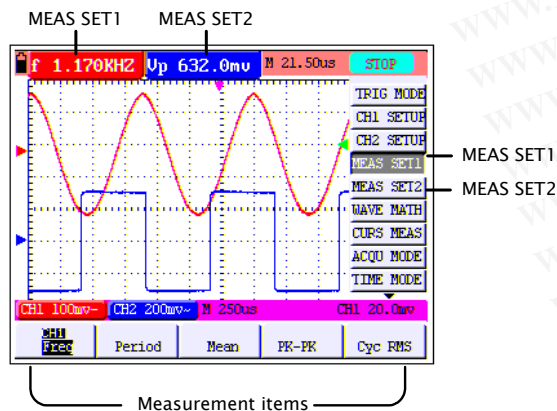

3. Select the measurement type from F1 (Freq) to

F5 (Cyc). Press it repeatedly to select CH1 or 2.

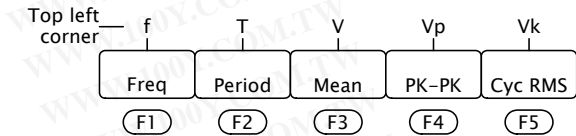

4. The measurement result appears in the top left corner of the display.

Running time cursor measurements


Overview The time cursor function measures and updates the following three types of time difference.

- Between cursor 1 and cursor 2
- Between cursor 1 and center (zero) point
- Between cursor 2 and center (zero) point


Time cursor panel operations

1. Make sure that the waveform appears.

2. Press the MENU key and select the CURS MEAS menu using the Up/Down keys.



3. Press F1 (Type) repeatedly to select the Time cursor. The cursors appear as vertical purple lines located at the center of the display.




4. Press the OSC OPTION key repeatedly until the following menu appears.

◀/▶ - Time


▲/▼ - Cursor 1(or 2)



5. Use the arrow keys to move the cursor or horizontal position.

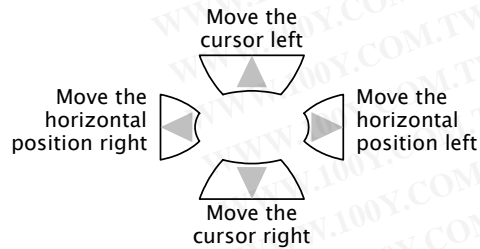

Display overview
(CH1, cursor 2)

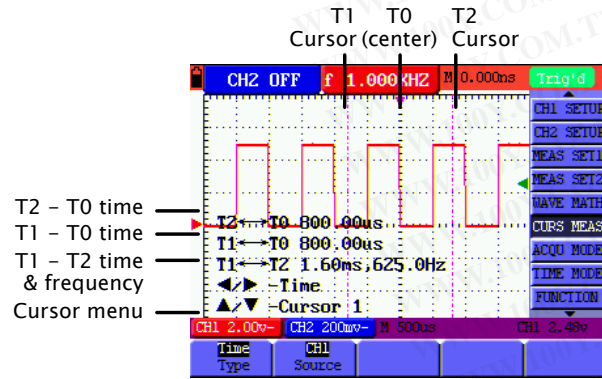

Running voltage cursor measurements


Overview The voltage cursor function measures and updates the following five types of voltage difference.

- Between cursor 1 and cursor 2
- Between cursor 1 and CH1 center point
- Between cursor 2 and CH1 center point
- Between cursor 1 and CH2 center point
- Between cursor 2 and CH2 center point

Source signal CH1 input, CH2 input

Voltage cursor panel operations 1. Make sure the waveform appears.

2. Press the MENU key and select the CURS MEAS menu using the Up/Down keys.



3. Press F1 (Type) repeatedly to select the Voltage cursor. The cursors appear as horizontal purple lines located at the center of the display.

Voltage Type
(F1)

4. Press F2 (Source) repeatedly to select the source channel.

CH1 Source
(F2)

5. Press the OSC OPTION key repeatedly until the following menu appears.


OSC OPTION

◀/▶ - Time


▲/▼ - Cursor V1 (or V2)



6. Use the arrow keys to move the cursor or horizontal position.

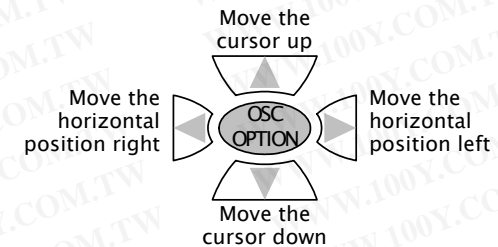

Display overview
(CH1, cursor 2)

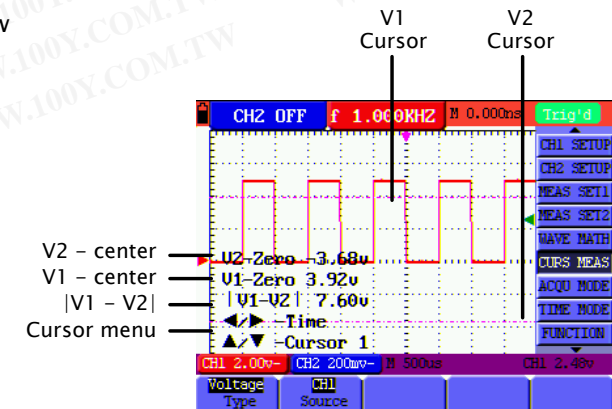

Advanced Viewings

Overview The advanced viewing functions allow you to clearly observe specific type of waveforms and/or particular characteristics in a waveform.


Viewing items	• Waveform zoom	page45
	• X-Y format	page47
	• Signal peaks	page48
	• Noisy signals	page48
	• Variations in a signal	page49

Zooming waveforms horizontally


Overview By using the zoom function, you can magnify the waveform in the horizontal direction.

Panel operations 1. Make sure that the waveform appears in the display.


2. Press the MENU key and select the TIME MODE menu using the Up/Down keys.



3. Press F2 (Set Window). A set of cursors appears in the center of the display.



Zoom window → ←

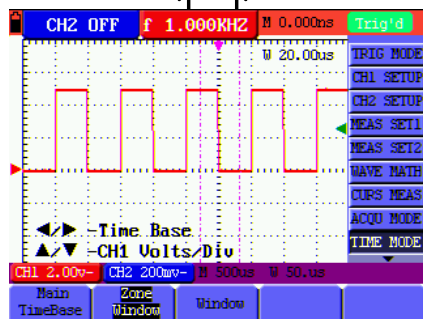

4. Press the OSC OPTION key repeatedly until the Time Base menu appears.




◀/▶ - Time

▲/▼ - Cursor V1


(or Cursor V2)




5. Use the arrow keys to change the zoom width.

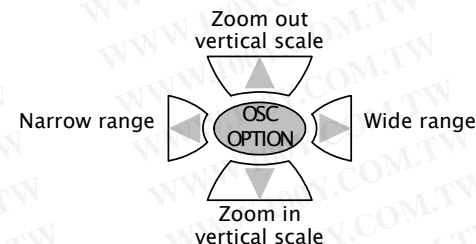

6. Press F3 (Window) to zoom into the window.



Example

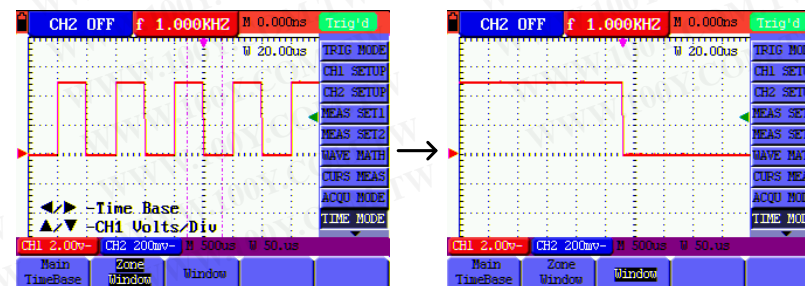


Viewing waveforms in X-Y format


Overview The X-Y format plots the CH1 input as X-axis and CH2 input as Y-axis. This display mode is convenient for viewing the phase relationship between CH1 and CH2.

Panel operations 1. Make sure that both CH1 and CH2 waveforms appear in the display.

2. Press the MENU key and select the DISP SET menu using the Up/Down keys.



3. Press F3 (Format) and select XY. The display mode switches into the X-Y format.



Changing the scale and position

Press the OSC OPTION key repeatedly to access the menu listed below. In the X-Y mode, all scales and positions are controlled by the Up/Down keys.



- CH1 Zero: horizontal position
- CH2 Zero: vertical position
- CH1 Vol: horizontal scale
- CH2 Vol: vertical scale

Functions not applicable in the X-Y format

The following functions do not work in the X-Y format.


- Cursor measurement (page42, page43)
- Automatic measurement (page41)
- Window zoom (page45)
- Trigger settings configuration (page25)

Viewing signal peaks

Overview Using the peak detect acquisition mode, the maximum and minimum data in the sampling interval are displayed, capturing the rapid changes and sudden peaks that might spontaneously occur in a waveform.


Note Since the peak detect mode picks up the most extreme data, the waveform becomes noisier than the normal acquisition mode (sampling mode).

- Panel operations** 1. Press the MENU key and use the Up/Down keys to select ACQU MODE menu.
2. Press F2 (Peak Detect) to activate the peak detect mode.

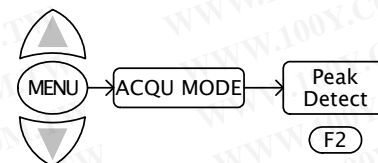

For other acquisition settings details, see page30.

Example

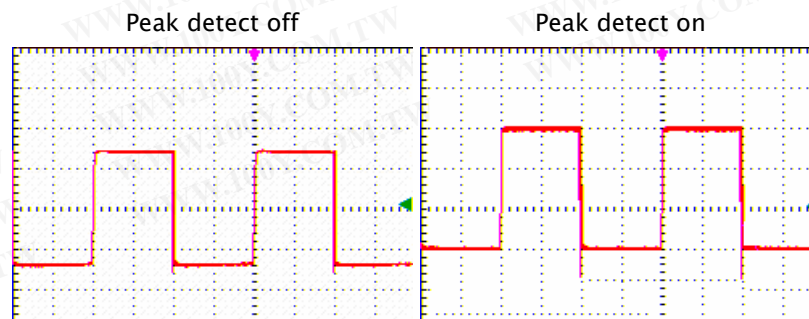


Viewing noisy signals

Overview Using the Average acquisition mode, you can smooth out the displayed waveform by averaging multiple data samples. The number of averaging is selectable from 4, 16, 64, and 128.


- Note**
- In order for the average mode to work in the best way, the waveform must be repetitive.
 - As the number of averaging increases, the slower the waveform update becomes.

- Panel operations**
1. Press the MENU key and use the Up/Down keys to select ACQU MODE menu.
 2. Press F3 (Average) to activate the average mode.
 3. Press F4 (Averages) repeatedly to select the number of averaging.

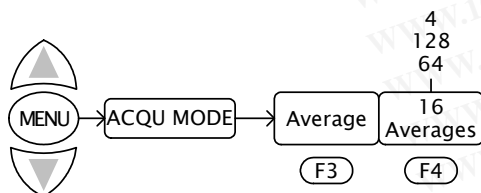

For other acquisition settings details, see page30.


Example

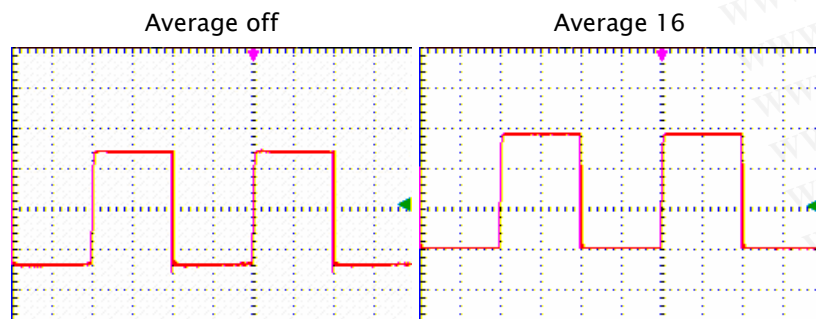

Viewing variations in a signal


Overview Using the persistence display function, you can define sets how long the old waveforms remain in the display, allowing observation of waveform variations. You can select the persistence time from 1, 2, and 5 sec. When choosing the Infinite mode, the GDS-122 keeps all past traces of the displayed waveform.

- Panel operations**
1. Press the MENU key and use the Up/Down keys to select DISP SET menu.
 2. Press F2 (Persist) repeatedly to select the persistence time.

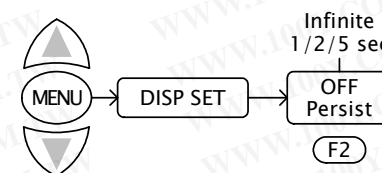

For other display settings details, see page36.

Example

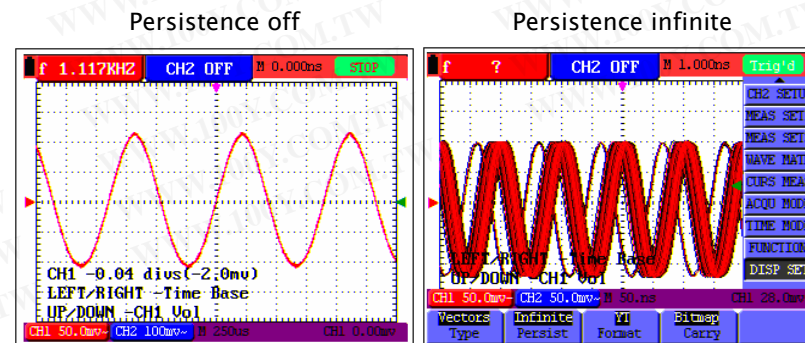

Calibration

Overview	The self calibration automatically adjusts the GDS-122 internal parameters. The probe calibration adjusts the probe capacitance. You should run both whenever using the GDS-122 in a new environment.
----------	---

Running the self calibration

Overview	The self calibration function automatically configures internal parameters to maintain the sensitivity and accuracy. Run the self calibration in the following cases.
----------	---

- When the temperature fluctuates more than 5 degrees Celsius during operations
- When operating the GDS-122 in a new benchtop or field environment

Procedure	<ol style="list-style-type: none"> 1. Press the MENU key and select the FUNCTION menu using the Up/Down keys. <div data-bbox="784 750 985 893"> </div> 2. Press F2 (Autocalibration). A message appears on the display, asking you to remove all cables and probes from the GDS-122. <div data-bbox="784 909 896 1021"> </div> 3. After removing all cables, press F2 (Autocalibration) again. The self-calibration automatically starts and a message appears, showing that the calibration is ongoing. <div data-bbox="784 1069 896 1181"> </div> 4. When the message disappears in 5 minutes, the calibration is completed.
-----------	---


To interrupt calibration	Press any key during the calibration.
--------------------------	---------------------------------------

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)



Running the probe calibration

Overview	The attached probe contains a calibration point at the end to adjust the waveform.
----------	--

Procedure	<ol style="list-style-type: none"> 1. You may use the GDS-122's own 1kHz square wave output signal. Insert the signal cable (included in the package) to the output terminal. <div data-bbox="1881 279 2038 462"> </div> 2. Use the Autoset function to put the waveform in the middle of the display. <div data-bbox="1881 478 1993 526"> </div>
-----------	---

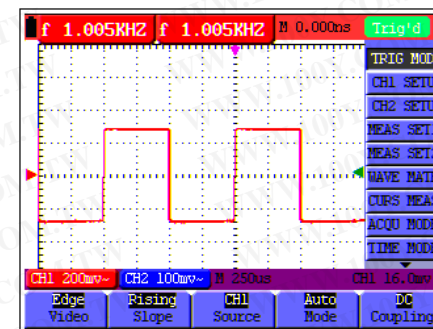

3. Adjust the probe calibration point to make sure that the waveform edge remains flat.

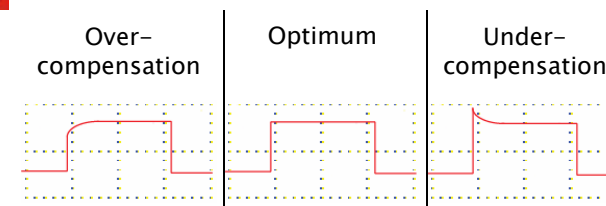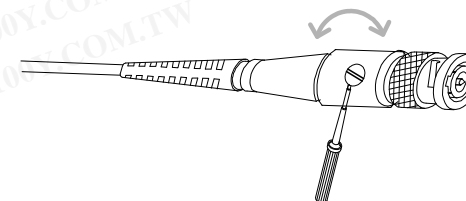

Saving/Recalling Waves and Settings


Overview The GDS-122 can save or recall four sets of waveforms using its internal memory. When you need to reset the system, recall the default (factory installed) settings.

Save/recall items

- Recalling default settings page53
- Saving waveforms page54
- Recalling waveforms page55

Recalling the default settings

Recalling the default settings You can recall the default factory settings by pressing the MENU key, then selecting FUNCTION → F1 (Recall Factory).

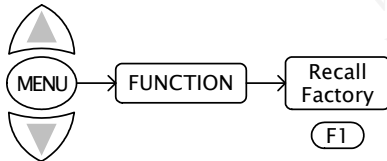

Trigger	Type: Edge Source: CH1 Coupling: AC	Slope: Rising Mode: Auto
CH1 & CH2	Coupling: AC Probe scaling: 1 X	Channel: ON Invert: OFF
Measurement 1	Item: CH1 frequency	
Measurement 2	Item: CH2 frequency	
Cursor	Cursor: OFF	Channel: CH1
Acquisition	Mode: Sample	Average number: 16
Time mode	Mode: Main timebase	
Display	Type: Vector Format: YT	Persistence: OFF Carry: Bitmap
Wave Save	Source: CH1 Display: OFF	Waveform: A

Saving waveforms

Overview Up to four waveforms can be stored in and recalled from the GDS-122 internal memory. The stored waveform can be used for reference, comparison, or analysis.


Memory Four memories: waveform A, B, C, and D.

Source CH1, CH2, Math waveform


Panel operations

1. Make sure the waveform you want to save (CH1, CH2, or Math result) appears in the display. For Math operations details, see page39.


2. Press the MENU key and select the WAVE SAVE menu using the Up/Down keys.




3. Press F1 (Source) repeatedly and select the waveform source.



4. Press F2 (WAVE) repeatedly and select the memory location from A to D.



5. Press F3 (Save) to confirm saving the waveform into the specified memory location. Make sure that the message "WAVE SAVED" appears in the display.




WAVE SAVED

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)


Recalling waveforms

Overview	Up to four waveforms can be stored in and recalled from the GDS-122 internal memory. The stored waveform can be used for reference, comparison, or analysis.
Memory	Four memories: waveform A, B, C, and D.
Source	CH1, CH2, Math waveform



- Panel operations
1. Press the MENU key and select the WAVE SAVE menu using the Up/Down keys.



2. Press F2 (Wave) repeatedly and select the waveform you want to recall.



3. Press F4 to turn on the waveform. The waveform appears in the display.

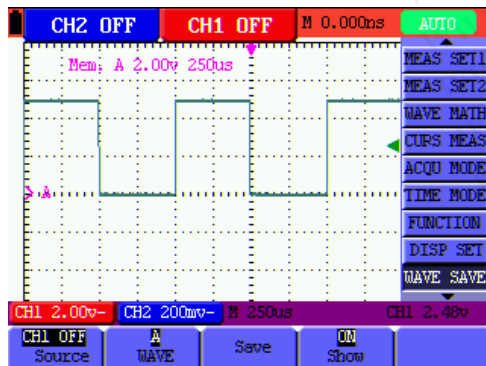

Note The recalled waveform maintains its original horizontal scale and vertical scale, which are shown in the top left corner of the display. Changing the current scale does not affect the recalled waveform's shape.

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)


Menu Tree / Operation Shortcuts

Accessing menus

The following menu trees are accessible by pressing the MENU key followed by Up/Down keys, except for the OSC OPTION key (page60).




Trigger

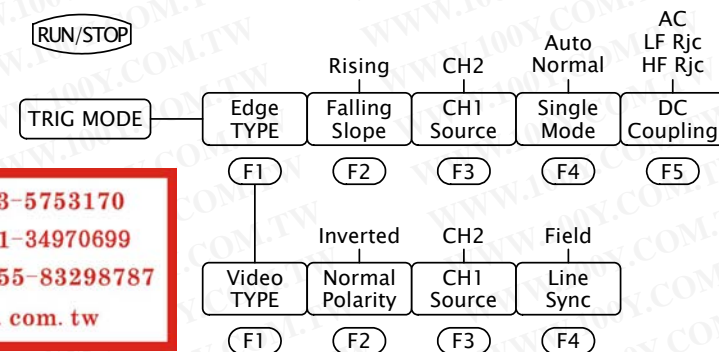

Select run or stop mode	RUN/STOP key
Select edge or video trigger	TRIG MODE→F1(TYPE)
Select trigger slope	TRIG MODE→F1(edge)→F2(Slope)
Select trigger source	TRIG MODE→F1→F3(Source)
Select trigger mode	TRIG MODE→F1(edge)→F4(Mode)
Select trigger coupling	TRIG MODE→F1(edge)→F5(Coupling)
Select video polarity	TRIG MODE→F1(video)→F2(Polarity)
Select video line sync	TRIG MODE→F1(video)→F4(Sync)


CH1/CH2 Setup

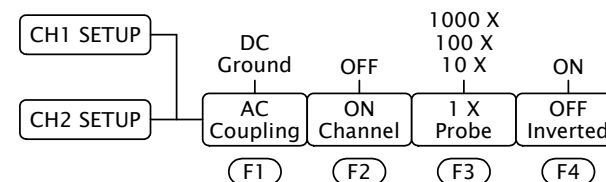

Select AC, DC, or Ground coupling	CH1/2 SETUP→F1(Coupling)
-----------------------------------	--------------------------


Turn CH1 on or off	CH1 /2 SETUP→F2(Channel)
Select probe scaling	CH1 /2 SETUP→F3(Probe)
Turn inversion on or off	CH1 /2 SETUP→F4(Inverted)

Measurement Setup 1/2

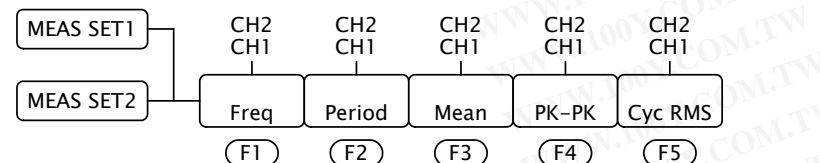


Measure CH1 /CH2 frequency	MEAS SET1 /2→F1(Freq)
Measure CH1 /CH2 period	MEAS SET1 /2→F2(Period)
Measure CH1 /CH2 mean value	MEAS SET1 /2→F3(Mean)
Measure CH1 /CH2 peak to peak time	MEAS SET1 /2→F4(PK-PK)
Measure CH1 /CH2 cycle	MEAS SET1 /2→F5(Cyc RMS)

Wave Math



Subtract CH2 from CH1	WAVE MATH→F1(CH1-CH2)
Subtract CH1 from CH2	WAVE MATH→F2(CH2-CH1)
Add CH2 to CH1	WAVE MATH→F3(CH1+CH2)
Multiply CH2 with CH1	WAVE MATH→F4(CH1*CH2)
Divide CH1 by CH2	WAVE MATH→F5(CH1/CH2)


Cursor Measurement

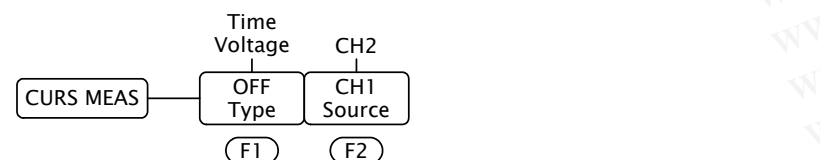

Activate cursor measurement	CURS MEAS→F1(Type)
Select source channel	CURS MEAS→F2(Source)


勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Acquisition Mode

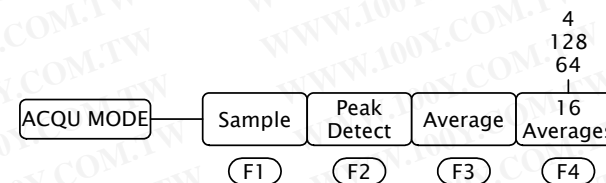


Select sampling mode	ACQU MODE→F1(Sample)
Select peak detect mode	ACQU MODE→F2(Peak Detect)
Select average mode	ACQU MODE→F3(Average)
Select average number	ACQU MODE→F3→F4(Averages)

Time Mode




Select main timebase	TIME MODE→F1(Main TimeBase)
Set window zoom width	TIME MODE→F2(Zone Window)
Zoom window	TIME MODE→F3(Window)

Function



Recall factory settings	FUNCTION→F1(Recall Factory)
Run self calibration	FUNCTION→F2(Autocalibration)

Display

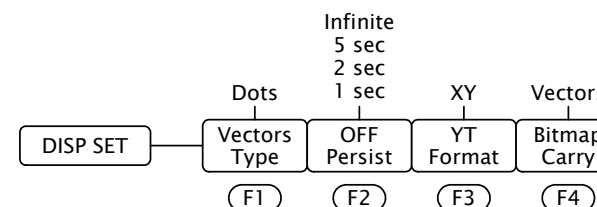

Select line display	DISP SET→F1 (Type)
Select persistency	DISP SET→F2 (Persist)
Select display format	DISP SET→F3 (Format)
Select display save format	DISP SET→F4 (Carry)

Wave Save


WAVE SAVE	Math CH2 CH1 Source (F1)	D C B A Wave (F2)	Save (F3)	ON OFF Show (F4)
Select source channel	WAVE SAVE→F1 (Source)			
Select waveform ID	WAVE SAVE→F2 (Wave)			
Save waveform	WAVE SAVE→F3 (Save)			
Turn waveform display on or off	WAVE SAVE→F4 (Show)			

System Status

SYS STAT	Horizontal (F1)	Vertical (F2)	Trigger (F3)	Misc (F4)
Show horizontal settings	SYS STAT→F1 (Horizontal)			
Show vertical settings	SYS STAT→F2 (Vertical)			
Show trigger settings	SYS STAT→F3 (Trigger)			
Show serial number	SYS STAT→F4 (Misc)			


勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

OSC OPTION key



Press the OSC OPTION key repeatedly. The menu message appears in the lower half of the display and the functionalities of four keys, UP, DOWN, RIGHT, LEFT, change accordingly.

LEFT/RIGHT - Time Base
 UP/DOWN - CH1 Vol

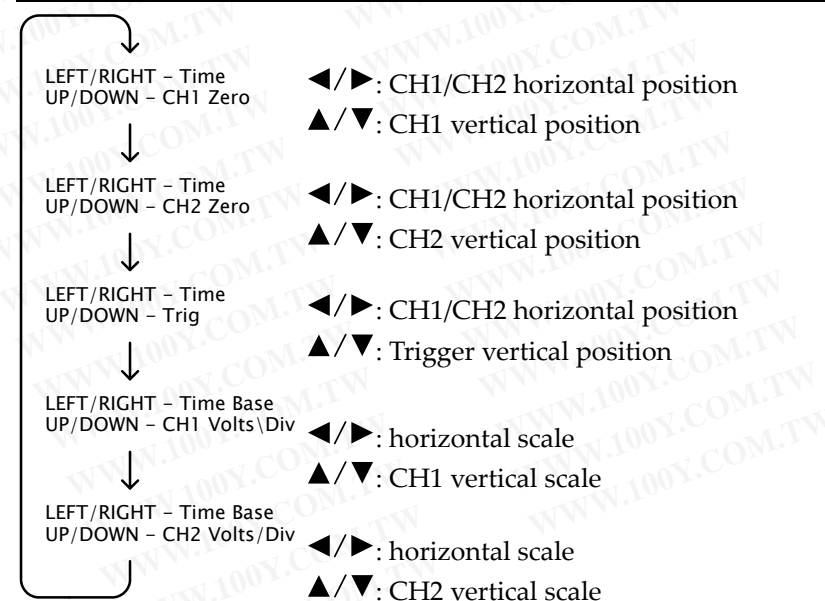

(Math mode)
 ◀/▶ - Time
 ▲/▼ - CHMath Volts/Div
 (Math mode)
 ◀/▶: Math horizontal position
 ▲/▼: Math vertical position

(Cursor mode)
 ◀/▶ - Time
 ▲/▼ - Cursor 1/2
 (Cursor mode)
 ◀/▶: CH1/CH2 horizontal position
 ▲/▼: Cursor 1/2 vertical position

Using the Software

Overview The GDS-122 PC software, included in the CD-ROM, allows you to view the waveforms in your familiar PC environment – large display and mouse operation. Multiple cursors provide flexible waveform measurements.

Software functionalities The PC software can run the following measurement and actions.

- Viewing real-time updated waveforms
- Running up to 6 cursor measurements
- Measuring period/frequency/pk-pk voltage
- Printing out waveform images
- Saving and recalling waveform shape and data

Software operations The following is the list of software operations described in this chapter.

- | | |
|---|--------|
| • Installing the software | page62 |
| • Modifying, reinstalling, or uninstalling the software | page64 |
| • Connecting the GDS-122 | page65 |
| • Configuring the screen | page68 |
| • Viewing waveforms | page69 |
| • Measuring waveforms | page75 |
| • Saving waveforms | page75 |
| • Recalling waveforms | page77 |
| • Printing out waveforms | page80 |
| • Accessing the Help | page82 |

Note The PC software is intended for oscilloscope operations only; it does not include multimeter operations.

Installing the software

- PC requirements**
- Windows 2000 or XP
 - 20MB hard drive space
 - USB host port x 1

Installation steps 1. Activate the Setup.exe file in the CD-ROM.




2. The language selection window appears. Select the software language and click **OK** (you can later change the language manually).

English

Simplified Chinese

英語 (美國)

Chinese (Simplified)

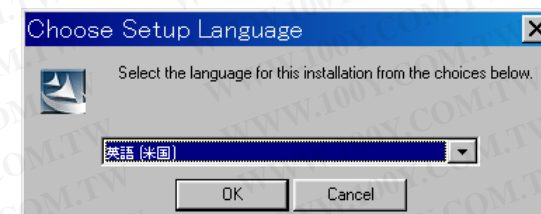


3. The software starts preparing the installation. When the welcome window is displayed, click **Next** and start installing the software to your PC.




4. The customer information window will appear. Enter the user name and organization name. Select which user will hold the right to access the software and click **Next**.


勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

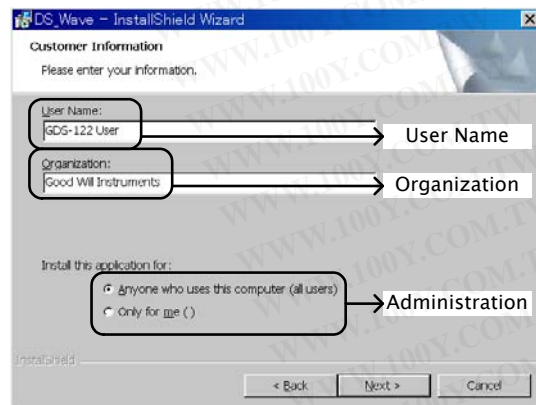

5. Change the installation directory if necessary and click *Next*.

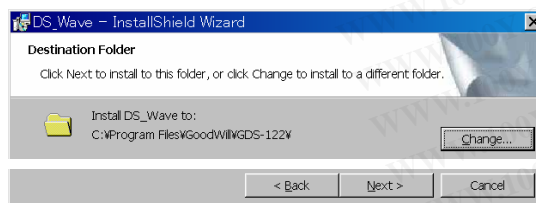

6. Click *Install* to start installing the software.

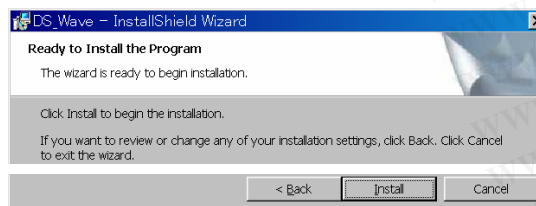

7. The software installation automatically starts and ends. Click *Finish* to complete installation.



Installing the software is completed

Modifying/Reinstalling/Uninstalling the software


Overview

After installing the software, you can do the followings using the same setup file.

- Modifying the software components
- Repairing the software
- Uninstalling the software

Steps


1. Activate the Setup.exe. Follow the same procedures as installing the software until the *Program Maintenance* window appears.

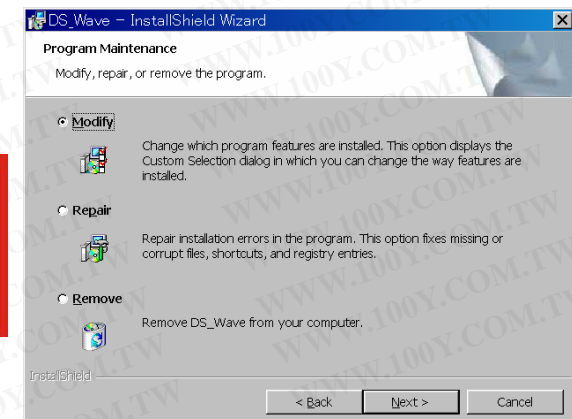

2. Select the action – *Modify* the software components, *Repair* the software, or *Remove* (uninstall) the software – and click *Next*. Proceed according to the instructions.

Shortcut for uninstall

Alternatively, you can select the Uninstall DC_Wave from the program startup menu to uninstall the software.

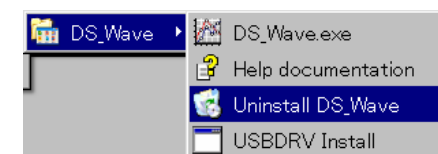

Activating the software and connecting the GDS-122


Overview

Activate the software and connect the GDS-122 to it properly by going through these steps, described in the paragraphs that follow.


1. Activating the software and configuring the communication port
2. Activating the GDS-122 and configuring the data format
3. Connecting them together and if necessary, installing the USB driver
4. Acquiring waveform data to confirm that the communication is being secured

Activating the software


1. Open the software by selecting DS_Wave.exe from the startup menu.



2. Select Communications – Ports Settings from the menu or click the Ports-settings icon on the Toolbar.




Make sure that USB connection is being selected. The baud rate, stop bit, data bit, and parity settings are fixed.

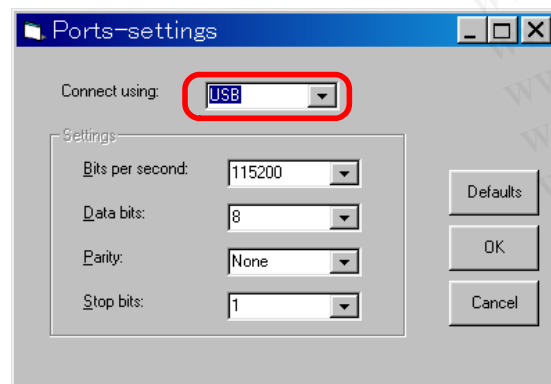

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Activating the GDS-122

1. Power up the GDS-122 and activate the oscilloscope screen.
2. Connect an input signal to CH1 and make sure that the waveform is shown appropriately on the GDS-122 display.
3. Open the DISP SET menu and press F4 (Carry) to select the format of the waveform data sent from the GDS-122 to the software.

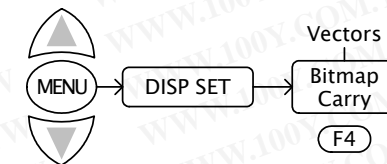


Vectors Vectored data of the waveform. Always select the vector format when viewing the waveform in the software.

Bitmap Bitmap image of the display. Select the Bitmap format only when taking the bitmap snapshot of the GDS-122 hardware screen.

Connecting the cable

1. Connect the GDS-122 to the PC (software) via the USB cable.
2. Make sure that the USB driver is installed in your PC by accessing the Device Manager (Control Panel -> System -> Hardware tab). The GDS-122 should be recognized as a USB hub.




3. If the driver has not been recognized, install it manually by selecting USBDRV Install from the startup menu.



The driver file is located in the USBDRV folder in the software directory.

Acquiring data

In the software, select Communications – Get Data from the menu. Alternatively, you may click the Get data icon, or press the Ctrl + A key.




Acquiring the GDS-122 display snapshot

When the “Bitmap” format is selected in the GDS-122 display carry setting, the software acquires the display snapshot (*.bmp) at the moment. Save the file in the local folder and use a graphic software to open and edit it.


Acquiring the GDS-122 waveform

When the “Vectors” format is selected in the GDS-122 display carry setting, the software acquires the waveform data (*.bin) at the moment.

1. The waveform data will be stored in the PC memory to allow to be recalled later (page79). Edit the location and click Start.

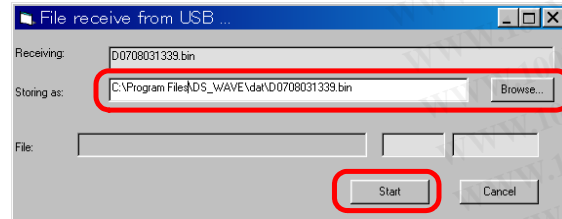

2. The waveform appears in the software screen.

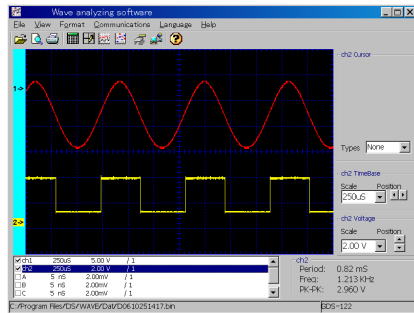

Connecting the GDS-122 to the software is completed


Configuring the screen

Overview

This section introduces how to configure the following parameters in the software screen (waveform viewing mode) to optimize the user interface.


- Background color
- Grid color
- Grid on/off
- Drawing format
- Language
- Closing the software

Screen overview

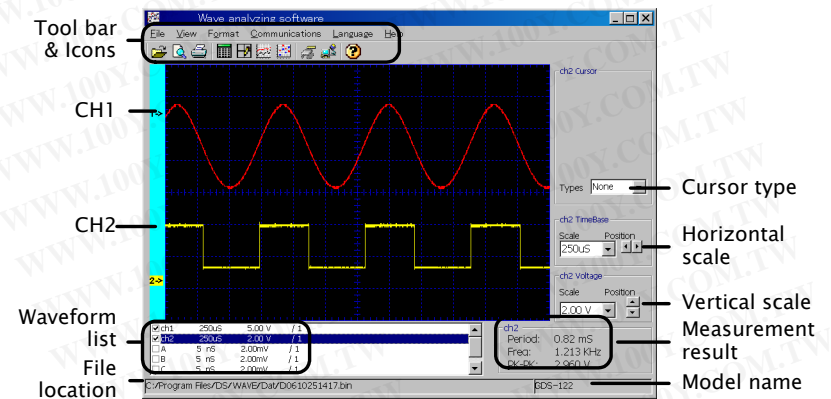


Changing the background color


To change the background color, select View > Background Color from the menu and select the new color from the color palette that appears. Alternatively, you can also double click inside the screen to call the color palette.



Black background




White background




勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Turning the grid on or off


To turn on or off the grid, select View > Grid lines from the menu or click the Gridlines icon.



Grid on




Grid off




Changing the grid color


Make sure the grid is already turned on. Select View > Grid Color from the menu and select the new color from the color palette that appears.



Blue grid





White grid





Changing the waveform drawing format

You can select how the waveform is being drawn from two formats, line and dots. Select Format > Data Line (Point) from the menu or click the icons.

Line



Point



Changing the language


You can select the language from English (default) or Simplified Chinese. Select Language > English (Chinese) from the menu. The Language menu itself always stays as English.



Closing the software

You can close the software in one of the following ways. The screen configurations will be retained the next time you open the software.

- Pressing the Alt + F4 keys
- Selecting File > Exit from the menu



- Clicking the Close icon at the top right corner of the software



勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)


Viewing the waveforms

Overview

This section introduces how to modify the waveform settings for better viewings.

- Selecting the displayed waveforms
- Refreshing the waveforms
- Selecting the active waveform
- Changing the waveform positions
- Changing the waveform scales
- Viewing the automatic measurement results

Screen overview

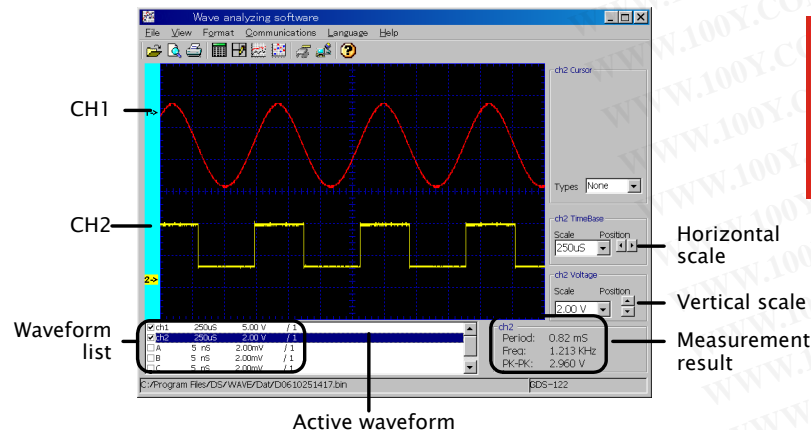

Selecting the displayed waveforms

In the left bottom corner of the screen, put a checkmark in the waveform that needs to appear. Maximum six waveforms are available: CH1, CH2, A, B, C, D. Waveforms A to D have to be stored in the GDS-122 hardware beforehand (see page54 for details).

(CH1, CH2 selected)

<input checked="" type="checkbox"/>	ch1	250uS	5.00 V	/ 1
<input checked="" type="checkbox"/>	ch2	250uS	2.00 V	/ 1
<input type="checkbox"/>	A	5 nS	2.00mV	/ 1
<input type="checkbox"/>	B	5 nS	2.00mV	/ 1
<input type="checkbox"/>	C	5 nS	2.00mV	/ 1

Refreshing the waveforms

In the software, select Communications – Get Data from the menu. Alternatively, you may click the Get data icon, or press the shortcut keys, Ctrl + A.



Selecting the active waveform

Waveform scale settings and automatic measurements are done on the active waveform.


1. Click on the waveform name in the bottom left corner of the screen.

(CH1 selected as the active waveform)

<input checked="" type="checkbox"/>	ch1	250uS	5.00 V	/ 1
<input checked="" type="checkbox"/>	ch2	250uS	2.00 V	/ 1
<input type="checkbox"/>	A	5 nS	2.00mV	/ 1
<input type="checkbox"/>	B	5 nS	2.00mV	/ 1
<input type="checkbox"/>	C	5 nS	2.00mV	/ 1

2. The following locations changes into the selected channel (example: CH1).

- Colored channel label (at the left side of the screen)
- Cursor, Time base, Voltage settings (at the right side of the screen)
- Automatic measurement results (at the bottom right corner of the display)



ch1 Cursor

ch1 TimeBase


ch1 Voltage

ch1	Period:	0.82 mS
	Freq:	1.213 KHz
	PK-PK:	13.200 V


Changing the waveform positions

Changing the horizontal position

1. Move the mouse over the waveform until the mouse icon changes into a left-right arrow.

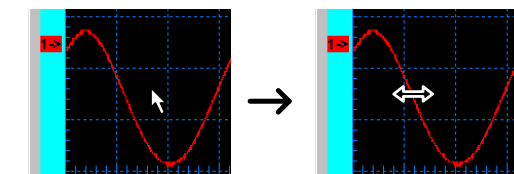


2. Hold the mouse and drag the waveform sideways.

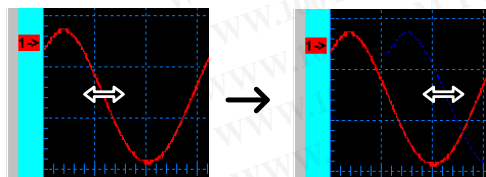

Changing the vertical position

Click the channel label at the left side of the waveform and drag the waveform up or down.

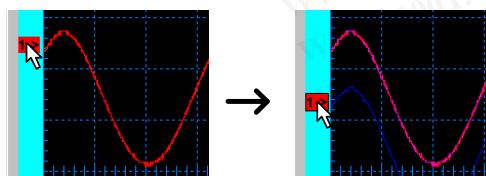



Changing the waveform scales

Before changing the scales, make sure that the correct waveform is selected (highlighted) in the lower left corner of the screen (example: CH1).





Changing the horizontal scale

Select the horizontal scale using the list at the right side of the screen. You can select the scale either by searching in the Scale column or by clicking the Position arrows.

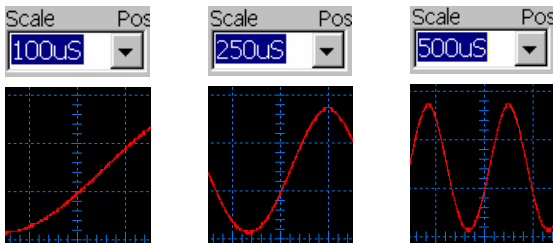


Changing the vertical scale

Select the vertical scale using the list at the right side of the screen. You can select the scale either by searching in the Scale column or by clicking the Position arrows.

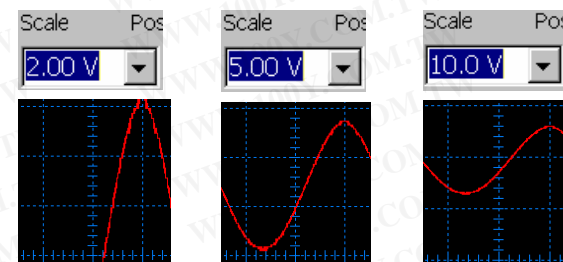

Viewing the automatic measurement results

Before viewing the measurement results, make sure that the correct waveform is selected (highlighted) in the lower left corner of the screen (example: CH1).



The measurement result is updated in the lower right corner of the screen. Three parameters are listed.



- Period: measures the waveform period in ms.
- Freq: measures the waveform frequency in kHz.
- PK-PK: measures the peak to peak voltage in V.


Using the cursor measurements

Overview

This section introduces how to use cursor measurements in the software screen.


- Activating the cursors
- Viewing the cursor measurement results
- Moving the cursors

Screen overview

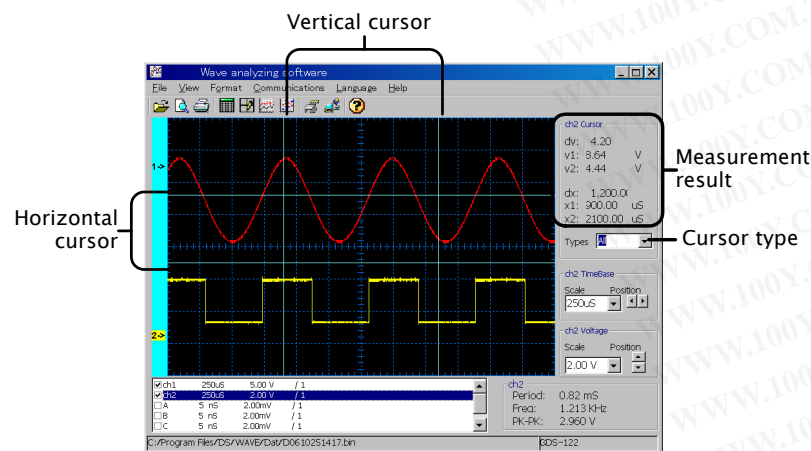

Activating the cursors

Before activating the cursors, make sure that the correct waveform is selected (highlighted) in the lower left corner of the screen (example: CH1).



Select the cursors from the list in the right side of the screen.


- None: the cursor is turned off. Types:
- Horizontal: the horizontal cursors appear. Types:
- Vertical: the vertical cursors appear. Types:

- All: both the horizontal and vertical cursors appear. Types:


Viewing the cursor measurement results

The cursor measurement results are updated in the right side of the screen.

- dy: the voltage difference between y1 and y2 cursors
- y1, y2: voltage cursors 1 and 2
- dx: the time difference between x1 and x2 cursors
- x1, x2: time cursors 1 and 2

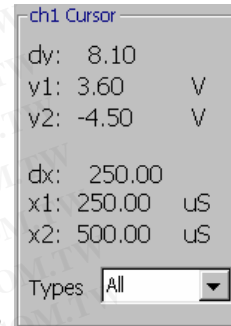


勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

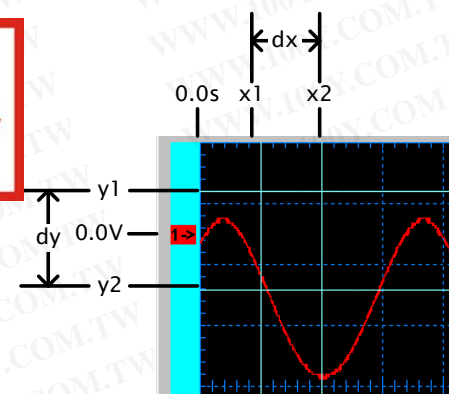

Moving the cursors

Move the mouse over the cursor until the mouse icon changes into a left-right arrow. Hold the mouse and drag the cursor sideways (horizontal cursor) or vertically (vertical cursor).

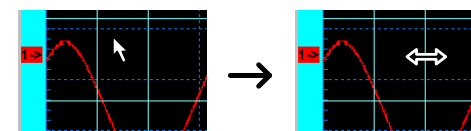

The cursor measurement result changes accordingly.

Saving waveforms

Overview

You can save the waveforms into the PC in two ways. For details of recalling them, see page79.

- Storing waveform data (*.bin file, for viewing in the software)
- Storing data points (*.txt file, for data analysis such as in graphs and maps)



For details of storing waveforms into the GDS-122 hardware, see page54.

Storing waveform data

When retrieving waveform data from the GDS-122, the waveform data (*.bin format) is automatically stored. For details, see page69.

Storing data point


1. Make sure that the waveform is being displayed in the screen. To recall waveforms that are stored in the PC, see page79.
2. Select **View > Data Table** from the menu, or click the Data Table icon on the Toolbar. The Data Table dialogue appears.

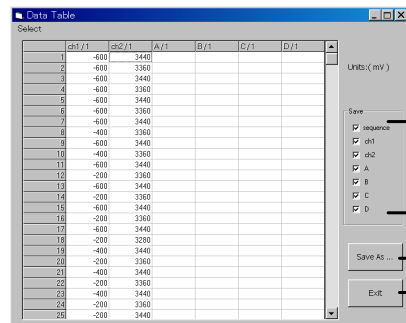

- Save option
- Save data
- Close window

3. Select the data to be saved from the Save column.


- sequence: the identification number for each data point
- ch1/ch2: CH1 and CH2 waveform data
- A/B/C/D: the waveforms stored in the GDS-122 hardware memory

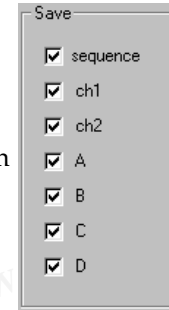

Data points stored in an Excel sheet (example)


	sequence	ch1 / ch2	A / B / C / D				
	A	B	C	D	E	F	G
1	Units: (mV)						
2	ch1 / 1	ch2 / 1	A / 1	B / 1	C / 1	D / 1	
3	1	-600	3440				
4	2	-600	3360				
5	3	-600	3440				
6	4	-600	3360				

4. Click the Save As... button to save the data into a directory. The standard Save dialog appears.



5. To close the Data Point dialogue, do one of the following actions.

- Press the Ctrl + Alt key
- Click the Exit icon



- Click the Close icon at the top right corner of the dialogue



Recalling waveforms

Overview



You can recall the waveforms from the PC in two ways. For details of saving them, see page 77.

- Recalling waveform data (*.bin file, for viewing in the software)
- Recalling data points (*.txt file, for data analysis such as in graphs and maps)

For details of recalling waveforms into the GDS-122 hardware, see page 55.

Recalling the waveform data

- Select **File > Open** from the menu or press the shortcut key, **Ctrl + O**.
- The File Open dialogue opens. Select one of the SPB bin file (*.bin) and click OK.
- The waveform(s) will be recalled in the screen.

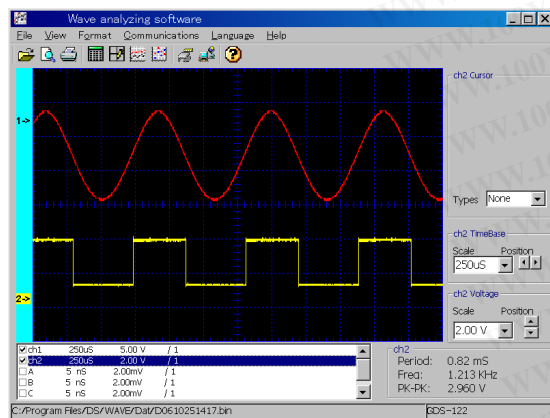

Recalling the data points

- For recalling the data points, you need to open a text editor or a spreadsheet program like Excel, in which you can organize the data and create graphs and maps for advanced analysis.
- Open the saved *.txt file from the application.

Printing out waveforms


Overview

You can print out the screen contents to a printer connected to the PC. When you are printing the waveform for the first time, follow all the steps in the following order.

- Setting up the printer
- Setting up the page format
- Printing out

Setting up the printer



- Select **File > Printer Setup** from the menu. The standard printer setting dialogue opens.



- Select the printer and its properties, paper size, and orientation.

Setting up the page format

- Select **File > Page Setup** from the menu. The Page Setup dialog window opens.

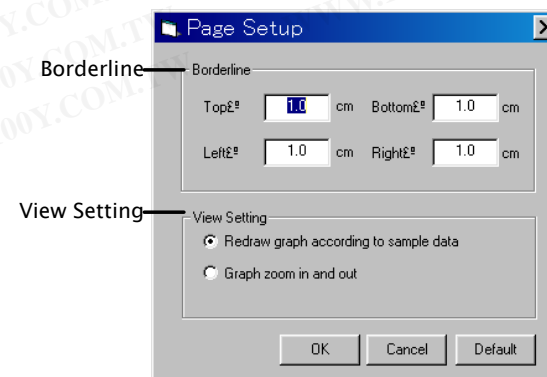

- Set the borderlines (print margins). The range is 0 to 10.0cm each.

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

3. Select the View Setting.


Redraw graph according to sample data:

The GDS-122 refreshes the waveform and adjust its scale before printing. The most recent data can be taken, but might take time for refreshing.

Graph zoom in and out

The existing waveform is used with its scale adjusted. Since retrieving the data is not involved, fast printing is ensured.


4. Open the print preview by selecting File > Print Preview from the menu or clicking the Print Preview icon on the toolbar. Make sure that the waveforms are placed appropriately.




Printing out

Print out the waveform in one of the following ways.

- Selecting File > Print in the Print Preview screen menu



- Selecting File > Print from the software menu



- Pressing the shortcut keys, Ctrl + P
- Clicking the Printer icon on the Toolbar




Accessing the Help

Overview The Help file describes how to install and use the software. The About screen shows the software version.

Opening the Help Open the Help in separate file using one of the following methods.

- Selecting Help > Help from the menu




- Clicking the Help icon on the Toolbar




- Pressing the shortcut key, F1

- Selecting the Help documentation from the startup menu

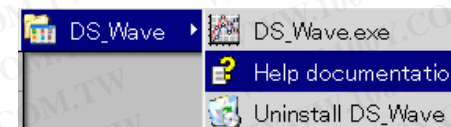

Software version To view the software version, select Help > About from the menu. The software version screen appears.



勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)








USING THE MULTIMETER

This chapter describes the multimeter functionalities in the GDS-122. Functionalities includes three major items (Voltage, Current, Impedance) and three additional items (Diode, Continuity, Capacitance). The current measurement and capacitance measurement use extension modules to deal with large current and small capacitance, respectively. Delta measurement and automatic range switching features offer flexibility and convenience.

Activating the Multimeter	84
Measuring Voltage	85
Measuring Current	87
Measuring Impedance	89
Measuring Diode	91
Measuring Continuity	92
Measuring Capacitance	93

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

Activating the Multimeter

- Panel operations
1. Press the power switch. The welcome screen with the corporate logo appears on the display. 
 2. To adjust display brightness, use the switch on the side: up (bright) or down (dark). 
 3. Press any key (example: MENU key) to activate the display. The battery icon at the top left corner of the display shows the battery level. (Example) 
 > 75% 75% 50% 25% < 25%

 4. Press A (current), V (voltage), or R (impedance, diode, continuity, capacitance) switch to proceed. A warning message might appear to remind you of correct connections. 






5. Press any key to cancel the warning message and resume the measurement.

Measuring Voltage


DC voltage specifications (details: page98)	Range	400mV, 4V, 400V
	Accuracy	$\pm(1\% + 1 \text{ digit})$
	Max input	400V

AC voltage specifications (details: page98)	Range	4V, 40V, 400V
	Accuracy	$\pm(1\% + 3 \text{ digits})$
	Max input	400V
	Frequency	40Hz to 400Hz


- Panel operations
- Press the V switch to select the Voltage measurement. If a warning message appears, press any key to resume measurement.
 - The voltage measurement screen appears.

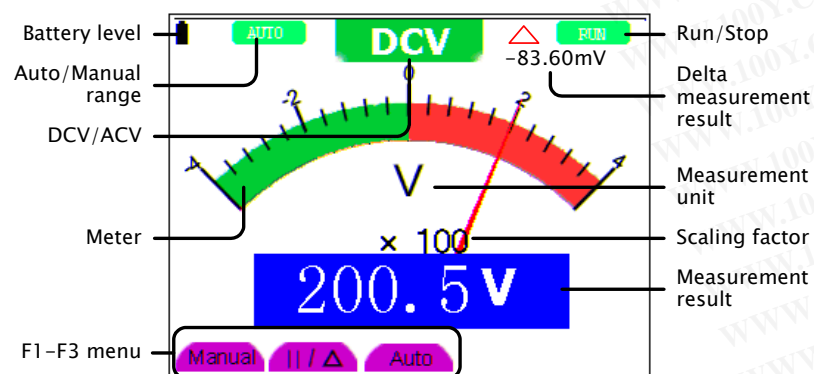

- Press the AUTOSET key repeatedly to select DC or AC voltage measurement.
- Connect the test leads to the terminals:
COM for the black lead
V/Ω/C for the red lead
- The measurement result will be constantly updated in the display. For more detailed settings, see the following instructions.



- | | | |
|--------------------------|---|--|
| Auto ranging | To let the GDS-122 select the voltage range automatically, press F3 (Auto). The indicator at the top left corner of the display changes to AUTO. | |
| Manual ranging | To select the voltage range manually, press F1 (Manual). The indicator at the top left corner of the display changes to MANUAL. | |
| Freezing the measurement | To freeze the measurement, press the RUN/STOP key. The measurement result will be retained and the indicator at the top right corner of the display changes to STOP. To unfreeze, press the RUN/STOP key again. | |
| Measuring delta voltage | To measure the delta value, press F2 (II/Δ). The measurement result at the moment moves to the top right corner of the display, and the measurement result becomes the difference between the original result. | |

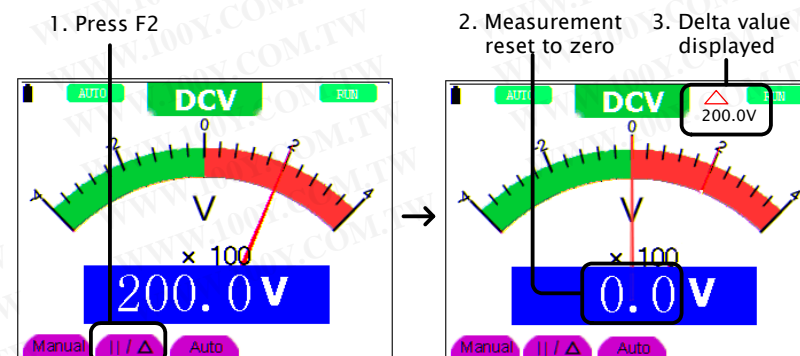


Measuring Current

DC current specifications (details: page98)	Range & Accuracy	40mA \pm (1% + 1 digit) 400mA \pm (1.5% + 1 digit) 20A \pm (3% + 3 digits)
	Max input	400mA (direct input) 20A (via the extension module)

AC current specifications (details: page98)	Range & Accuracy	40mA \pm (1.5% + 3 digits) 400mA \pm (2% + 1 digit) 20A \pm (5% + 3 digits)
	Max input	400mA (direct input) 20A (via the extension module)

- Panel operations 1. Press the A switch to select the current (Ampere) measurement. If a warning message appears, press any key to resume measurement.

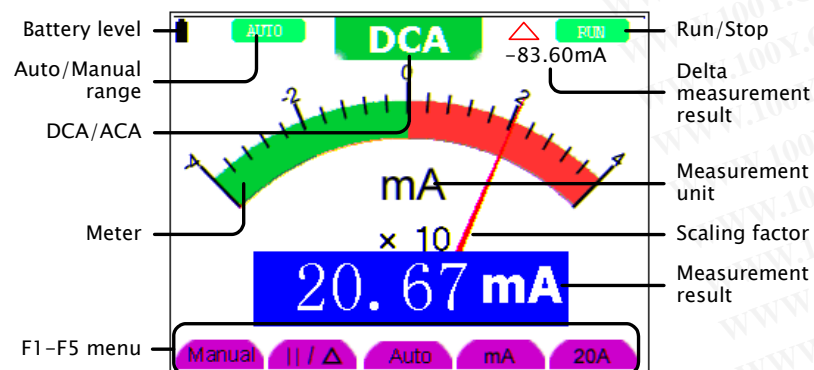


2. Press the AUTOSET key repeatedly to select DC or AC current measurement.




- Measuring 0mA to 400mA 1. Connect the test leads to the terminals: COM for the black lead mA/A for the red lead



If the range is set at 20A, press F4 (mA) and change it to mA range.




2. Select automatic range by pressing F3 (Auto) or manual by F1 (Manual). The indicator at the top left corner of the display changes accordingly.




Measuring 400mA to 20A



1. Connect the Current Extension module to the COM & mA/A terminals. Then, connect the test leads to the extension module.



2. Press F5 (20A) and select the 20A range. The MANUAL range indicator activates. (Auto range is not available)




Freezing the measurement

To freeze the measurement, press the RUN/STOP key. The measurement result will be retained and the indicator at the top right corner of the display changes to STOP. To unfreeze, press the RUN/STOP key again.





Measuring delta current

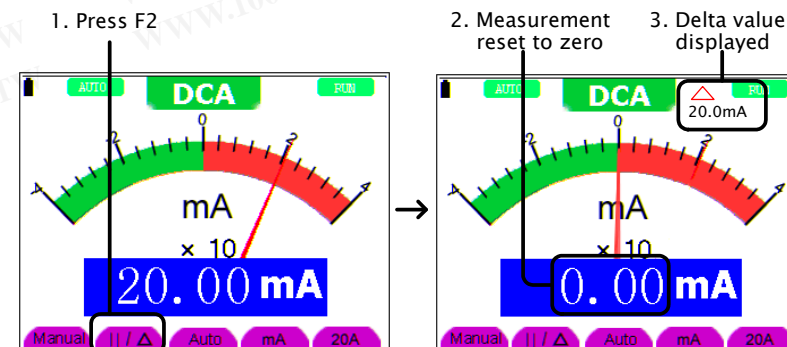
To measure the delta value, press F2 (II/Δ). The measurement result at the moment moves to the top right corner of the display, and the measurement result becomes the difference between the original result.




Measuring Impedance


Impedance specifications (details: page98)	Range & Resolution	400Ω ±(1% + 3 digits)
		4k, 40k, 400k, 4MΩ ±(1% + 1 digit)
		40MΩ ±(1.5% + 3 digits)


- Panel operations
1. Press the R switch. If a warning message appears, press any key to resume measurement. 
 2. Press the AUTOSET key repeatedly to select the impedance measurement. 
 3. The impedance screen appears.

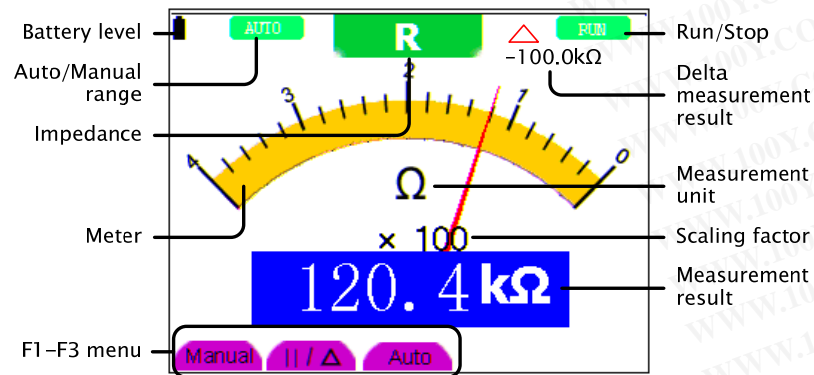



4. Connect the test leads to the terminals:
COM for the black lead
V/Ω/C for the red lead
5. The measurement result will be constantly updated in the display. For more detailed settings, see the following instructions.




- Auto ranging
- To let the GDS-122 select the voltage range automatically, press F3 (Auto). The indicator at the top left corner of the display changes to AUTO. 

- Manual ranging
- To select the voltage range manually, press F1 (Manual). The indicator at the top left corner of the display changes to MANUAL. 



- Freezing the measurement
- To freeze the measurement, press the RUN/STOP key. The measurement result will be retained and the indicator at the top right corner of the display changes to STOP. To unfreeze, press the RUN/STOP key again. 


- Measuring delta impedance
- To measure the delta value, press F2 (II/Δ). The measurement result at the moment moves to the top right corner of the display, and the measurement result becomes the difference between the original result. 

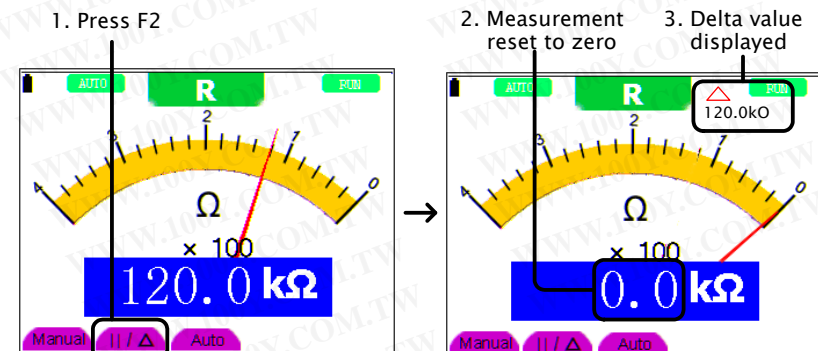


Measuring Diode

Range 0V to 1.5V

- Panel operations
1. Press the R switch. If a warning message appears, press any key to resume measurement. 
 2. Press the AUTOSET key repeatedly to select the diode measurement. 
 3. The diode measurement screen appears.

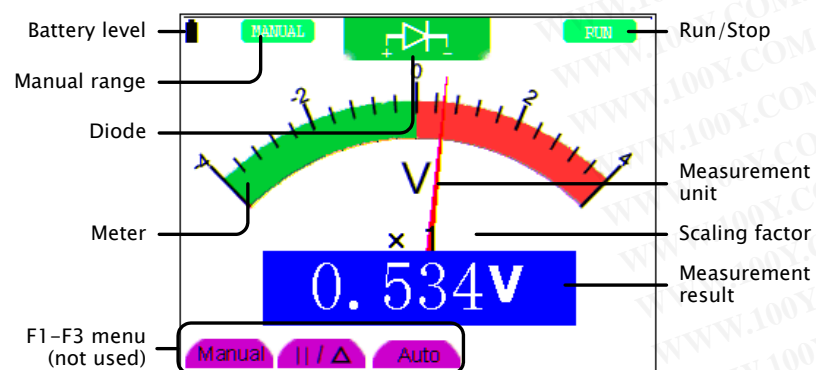

4. Connect the test leads to the terminals:
COM for the black lead
V/ Ω /C for the red lead
5. The measurement result will be constantly updated in the display.





- Freezing the measurement
- To freeze the measurement, press the RUN/STOP key. The measurement result will be retained and the indicator at the top right corner of the display changes to STOP. To unfreeze, press the RUN/STOP key again.




勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)


Measuring Continuity

Conditions < 50 Ω (beeping)

- Panel operations
1. Press the R switch. If a warning message appears, press any key to resume measurement. 
 2. Press the AUTOSET key repeatedly to select the continuity measurement. 
 3. The continuity measurement screen appears.

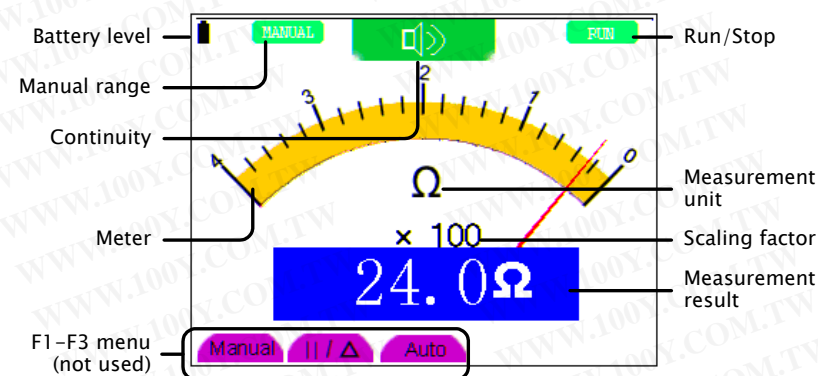

4. Connect the test leads to the terminals:
COM for the black lead
V/ Ω /C for the red lead
5. If the GDS-122 confirms continuity (the impedance is less than 50 Ω), the beeper sounds.






- Freezing the measurement
- To freeze the measurement, press the RUN/STOP key. The measurement result will be retained and the indicator at the top right corner of the display changes to STOP. To unfreeze, press the RUN/STOP key again.



Measuring Capacitance


Continuity specifications Range 51.2nF to 100uF $\pm(3\% + 3 \text{ digits})$

- Panel operations
1. Press the R switch. If a warning message appears, press any key to resume measurement.  $\Omega/\nabla/\Delta/C$
 2. Press the AUTOSET key repeatedly to select the capacitance measurement. 
 3. The capacitance screen appears.

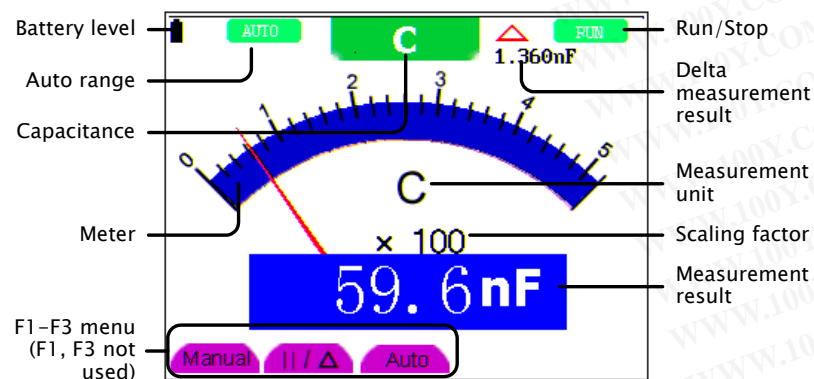

Measuring 5nF and above


Connect the test leads to the CX terminals.



Measuring less than 5nF



Connect the Capacitance Extension module to the COM & V/Ω/C terminals. Then, connect the test leads to the extension module. The measurement result will be constantly updated in the display.




Freezing the measurement

To freeze the measurement, press the RUN/STOP key. The measurement result will be retained and the indicator at the top right corner of the display changes to STOP. To unfreeze, press the RUN/STOP key again.



Measuring delta capacitance

To measure the delta value, press F2 (II/Δ). The measurement result at the moment moves to the top right corner of the display, and the measurement result becomes the difference between the original result.

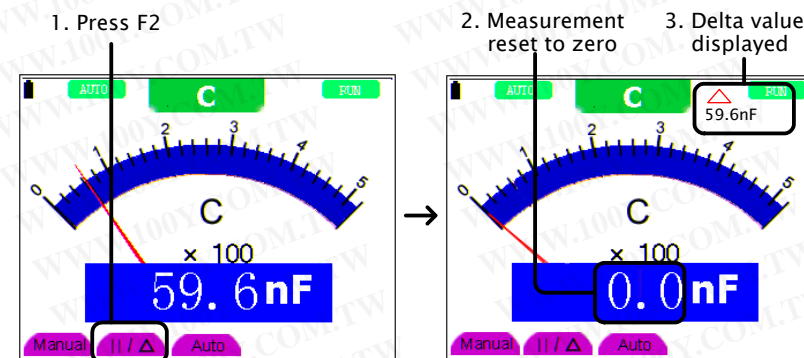

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

FAQ

Power

- Q • The GDS-122 does not power up.
• The GDS-122 stopped working after a short period of time.
- A The battery may need recharging. Connect the GDS-122 to the AC adaptor and recharge it for at least 15 minutes. Then try powering up.

ERR mode in the multimeter

- Q In the multimeter mode, the measurement type at the top of the display says "ERR" which looks like an error message.
- A The "ERR" sign appears when none of the measurement switch is pressed. Select one from the V, A, or R switch and press it.

Amplitude mismatch in the oscilloscope

- Q The measured voltage is 10 times smaller than the real value.
- A The attenuation ratio on the probe is set at x10. If you switch it to x1, make sure that the input voltage does not surpass the maximum 400V.
- Q The measured voltage is 10/100/1000 times larger than the real value.
- A The probe ratio in the CH1 or CH2 setup menu is set at X10, X100, or X1000. See page22 for details.

Unstable waveform in the oscilloscope

- Q The waveform appears in the display but is not stable.
- A Configuring the trigger might help you. See page30 for details.
- Make sure the trigger source channel matches the input signal.
 - Make sure the correct trigger type, edge or

video, is selected.

- Try changing the HF and LF repression in the trigger coupling mode and filtering out high or low frequency noise.

No waveform in the oscilloscope

- Q The waveform does not appear at all in the display.
- A • The trigger level might be out of the waveform range. Press the AUTOSET key so that the GDS-122 automatically adjusts the trigger level.
• If the trigger mode is Single, press the RUN/STOP key to trigger the waveform or switch the trigger mode to Normal. See page30 for trigger details.

Slow update in the multimeter

- Q It takes 30 to 40 seconds for the multimeter to update the capacitor measurement.
- A It takes longer time to measure small capacitors. 30 to 40 seconds are normal for measuring 5nF or smaller capacitors. See page93 for capacitance measurement details.

Slow update in the oscilloscope

- Q The display response to the waveform change is unusually slow.
- A Slow response is normal in the following cases.
- Average sampling mode is being selected (page22)
 - Display persistence is being selected (page36)

SPECIFICATIONS

Conditions for specifications

The following specifications are applicable when these two conditions are met:

- The GDS-122 has been powered up for at least 30 minutes, during which temperature fluctuation is no more than 5 degrees Celsius.
- The probe attenuation is set to X 10.

Oscilloscope specifications

Sampling	Mode	Normal, Peak detection, Average
	Rate	100 MSa/s
Input	Coupling	DC, AC
	Impedance	1M Ω ±2% in parallel with 20pF±3pF
	Probe	1X, 10X, 100X, 1000X
	Max. Input	400V (peak)
	Channel delay	150ps (typical)
Horizontal	Sampling rate	10S/s~100mS/s
	Interpolation	(sin x) /x
	Record length	6K points on each channel
	Scanning speed	5ns/div~5s/div, 1-2.5-5 step
	Sampling rate / relay time accuracy	±100ppm (time interval ≥ 1ms)
	Interval (ΔT) accuracy (full bandwidth)	Single: ±(1 interval time +100ppm×reading+0.6ns) Average >16 : ±(1 interval time +100ppm×reading+0.4ns)
	Interval (ΔT) accuracy (full bandwidth)	Single: ±(1 interval time +100ppm×reading+0.4ns)
Vertical	A/D converter	8 bits resolution (2CH simultaneously)
	Sensitivity	5mV/div~5V/div (at input)
	Displacement	±50V(500mV~5V), ±1V(5mV~200mV)
	Bandwidth	20M
	Single	Full bandwidth
	Low frequency	≥5Hz (at input, AD coupling, -3dB)
	Rise time	≤17.5ns (at input, typical)
	DC accuracy	±5% (DC gain)
	DC accuracy (avg)	Avg >16: ±(5% rdg + 0.05 div) for ΔV

Trigger	Sensitivity	CH1 and CH2: 1div(DC~full bandwidth) DC coupling: ≥ 50Hz.	
	Trigger level	±6 divisions from the screen center	
	Level accuracy	±0.3 div (typical, rise/fall time ≥ 20ns)	
	Displacement	655div (pre-trigger), 4div (post-trigger)	
	50% level setting	Input signal frequency ≥ 50Hz (typical)	
	Trigger sensitivity	2 div of peak-to-peak (video trigger)	
Measurement	Signal system	NTSC, PAL, SECAM (any frequency)	
	Cursor	ΔV and ΔT between cursors	
	Automatic	Peak-to-peak, average, root mean square, frequency, and cycle	
Probe		1X position	10X position
	Bandwidth	≤ 6 MHz (DC)	Full bandwidth (DC)
	Attenuation rate	1: 1	10: 1
	Compensation	10pf~35pf	10pf~35pf
	Input impedance	1M Ω ±2%	10M Ω ±2%
	Input impedance	85pf~115pf	14.5pf~17.5pf
	Input voltage	150 V DC	300V DC

Multimeter specifications

VDC	Input impedance	10M Ω
	Max input	1000V (DC or AC peak-to-peak value)
	Accuracy	±1%±1 digit
	Resolution	400mV range: 100uV 4V range: 1mV 40V range: 10mV 400V range: 100mV
	Resolution	400V range: 100mV
VAC	Input impedance	10M Ω
	Max input	750V(AC, virtual value)
	Frequency range	40Hz~400Hz
	Display	Virtual value of sine wave
	Accuracy	±1%±3 digits
DCA	Resolution	4V range: 1mV 40V range: 10mV 400V range: 100mV
	Accuracy	40mA range: ±1%±1 digit 400mA range: ±1.5%±1 digit 20A range: ±3%±3 digits
	Resolution	40mA range: 10uA
	Resolution	40mA range: 10uA
	Resolution	40mA range: 10uA

		400mA range: 100uA 20A range: 10mA
ACA	Accuracy	40mA range: $\pm 1.5\% \pm 3$ digit 400mA range: $\pm 2\% \pm 1$ digit 20A range: $\pm 5\% \pm 3$ digits
	Resolution	40mA range: 10uA 400mA range: 100uA 20A range: 10mA
Resistance	Accuracy	400Ω range: $\pm 1\% \pm 3$ digits 4kΩ~4MΩ range: $\pm 1\% \pm 1$ digit 40MΩ range: $\pm 1.5\% \pm 1$ digit
	Resolution	400Ω range: 0.1Ω 4kΩ range: 1Ω 40kΩ range: 10Ω 400kΩ range: 100Ω 4MΩ range: 1kΩ 40MΩ range: 10kΩ
Capacitance	Accuracy	$\pm 3\% \pm 3$ digits
	Resolution	51.2nF range: 10pF 512nF range: 100pF 5.12uF range: 1nF 51.2uF range: 10nF 100uF range: 100nF
Diode	Reading range	0V~1.5V
Continuity	Threshold	< 30Ω

General specifications

Display	Type	3.8" color liquid crystal display
	Resolution	320 (horizontal) × 240 (vertical) pixels
	Color	4096 colors
Power	Consumption	< 6W
	Supply	100V~240V AC, 50/60Hz
	DC input	8.5VDC, 1500mA
Environment	Operating	Temperature: 0 to 40 °C(32 to 104 °F) Relative humidity: < 75%
	Storage	Temperature: -20 to 60 °C(-4 to 140 °F) Relative humidity: < 75%
Mechanical	Dimension	18 cm×11.5cm×4cm
	Weight	690g

DECLARATION OF CONFORMITY

We

GOOD WILL INSTRUMENT CO., LTD.

(1) No.7-1, Jhongsing Rd., Tucheng City, Taipei County, Taiwan

(2) No. 69, Lu San Road, Suzhou City (Xin Qu), Jiangsu Sheng, China

declare, that the below mentioned product

Type of Product: Handheld Digital Storage Oscilloscope & Multimeter

Model Number: GDS-122

is herewith confirmed to comply with the requirements set out in the Council Directive on the Approximation of the Law of Member States relating to Electromagnetic Compatibility (89/336/EEC) and Low Voltage Directive (73/23/EEC).

For the evaluation regarding the Electromagnetic Compatibility and Low Voltage Directive, the following standards were applied:

© EMC

EN 61326-1: Electrical equipment for measurement, control and laboratory use — EMC requirements (1997 + A1:1998 + A2:2001 + A3:2003)

Current Harmonics

EN 61000-3-2: 2000 + A2:2005

Voltage Fluctuations

EN 61000-3-3: 1995 + A1:2001

© Safety

Low Voltage Equipment Directive 73/23/EEC

Safety Requirements

IEC/EN 61010-1: 2001 (2nd Edition)

勝特力材料 886-3-5753170
勝特力电子(上海) 86-21-34970699
勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

INDEX

勝特力材料 886-3-5753170
 勝特力电子(上海) 86-21-34970699
 勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)

AC coupling	channel
trigger	edge trigger
vertical	on/off
ACA multimeter	video trigger source
specifications	contents of package
AC-DC adaptor	continuity, multimeter
acquisition	specifications
short cuts	coupling
system status	system status
ACV multimeter	trigger
specifications	vertical
addition, math mode	cursor measurement
auto ranging	PC software
impedance multimeter	short cuts
voltage multimeter	time
auto trigger mode	voltage
AUTO trigger status	cycle rms, automatic measurement
automatic measurements	data point, storing
shortcuts	data table, PC software
Autoset	DC coupling
capacitance multimeter	trigger
continuity, multimeter	vertical
diode, multimeter	DCA multimeter
impedance measurement	specifications
voltage multimeter	DCV multimeter
average acquisition mode	specifications
application	default settings
background color, PC software	delta measurement
battery level	capacitance multimeter
calibration	current multimeter
short cuts	impedance multimeter
capacitance measurement,	voltage multimeter
multimeter	diode measurement, multimeter
specifications	specifications
carry, interface setting	display
carrying case	acquiring snapshot
caution symbol	brightness adjustment
CD-ROM	overview

settings	36	grid, PC software	69
shortcuts	58	ground symbol	6
specifications	99	help, PC software	82
division, math mode	39	Hf Rjc	32
dot drawing	36	horizontal	
edge trigger	30	adjusting position	20, 25
auto mode	31	adjusting scale	19, 26
coupling mode	32	scale vs trigger status	28
mode	31	short cuts	58
normal mode	32	specifications	97
single mode	32	system status	37
EN61000	100	impedance, multimeter	89
EN61010		specifications	99
declaration of conformity	100	installing PC software	62
measurement category	7	inverting channel	24
pollution degree	7	language	
EN61326-1	100	PC software	70
environment		short cuts	58
operation	7	LF Rjc	32
specifications	99	line data, PC software	69
storage	8	line trigger, video	34
ERR mode, multimeter	95	list of features	11
extension module		magnification, vertical	25
capacitance multimeter	93	manual ranging	
current multimeter	88	current multimeter	88
package	10	impedance multimeter	90
factory settings	53	voltage multimeter	86
FAQ	95	manual, overview of	14
ERR mode, multimeter	95	math mode	39
magnification	95	shortcuts	57
no waveform	96	system status	38
powering up	95	mean voltage, auto measurement	41
slow update, multimeter	96	multimeter	
slow update, oscilloscope	96	activating	84
unstable waveform	95	capacitance measurement	93
field trigger, video	34	continuity measurement	92
freezing measurement		current measurement	87
capacitance multimeter	94	diode measurement	91
continuity multimeter	92	ERR mode	95
current multimeter	88	impedance measurement	89
diode multimeter	91	specifications	98
impedance multimeter	90	voltage measurement	85
voltage multimeter	86	warning message	84
frequency, automatic measurement	41	multiplication, math mode	39
front panel overview	12	noisy signal, viewing	49
grid color, PC software	69	normal trigger mode	32

operation environment.....	7	calibration.....	52
OSC option key.....	60	package.....	10
oscilloscope		setting attenuation.....	17
specifications.....	97	specifications.....	98
switching to multimeter.....	16	Ready trigger status.....	27
package contents.....	10	recalling	
PC software		default settings.....	53
activation.....	65	default settings, shortcuts.....	58
cursor measurement.....	75	waveforms from GDS-122.....	55
help.....	82	waveforms, PC software.....	79
installation.....	62	resetting trigger level.....	29
overview.....	61	run trigger.....	28
package.....	10	sample acquisition mode.....	35
printing out.....	80	saving	
saving waveform.....	77	shortcuts.....	59
screen overview.....	68	waveforms in PC software.....	77
uninstall.....	64	waveforms inside GDS-122.....	54
version.....	82	scale	
viewing waveforms.....	71	horizontal.....	26
peak detect acquisition mode.....	35	math mode.....	40
application.....	48	vertical.....	23
period, automatic measurement.....	41	waveform, PC software.....	73
persistence setting.....	36	xy mode.....	47
application.....	50	zoom.....	46
pk-pk voltage, automatic		Scan trigger status.....	27
measurement.....	41	self calibration.....	51
point data, PC software.....	69	SET1/2, automatic measurement.....	41
position		signal peak, viewing.....	48
horizontal.....	25	single trigger mode.....	32
math mode.....	40	slope, trigger.....	30
shortcuts.....	60	snapshot, display.....	67
time cursor.....	43	software version.....	82
trigger.....	28	specifications	
vertical.....	23	general.....	99
voltage cursor.....	44	multimeter.....	98
waveform, PC software.....	72	oscilloscope.....	97
xy mode.....	47	stop trigger.....	28
power supply		STOP trigger status.....	27
safety instructions.....	7	storage environment.....	8
specifications.....	99	subtraction, math mode.....	39
power up, faq.....	95	synchronization, video trigger.....	34
powering up.....	16	system status.....	37
print out, PC software.....	80	shortcuts.....	59
probe		test lead.....	10
adjusting display magnification.....	17	threshold, continuity multimeter.....	92
adjustment tool.....	10	tilt stand.....	17

time cursor.....	42	variations, viewing.....	50
Trig'd trigger status.....	27	vector drawing.....	36
trigger		vertical	
adjusting level.....	28	adjusting position.....	20, 23
auto mode.....	31	adjusting scale.....	19, 23
channel, edge trigger.....	31	inverting channel.....	24
coupling mode.....	32	selecting coupling mode.....	24
edge triggering.....	30	selecting magnification.....	25
mode.....	31	shortcuts.....	56
normal mode.....	32	specifications.....	97
run/stop.....	28	system status.....	38
shortcuts.....	56	video trigger.....	33
single mode.....	32	field trigger.....	34
slope.....	30	line trigger.....	34
source channel, video.....	34	source channel.....	34
specifications.....	98	sync.....	34
status icons.....	27	voltage cursor.....	43
status vs horizontal scale.....	28	warning message, multimeter.....	84
sync, video trigger.....	34	warning symbol.....	6
system status.....	38	xy mode.....	47
video.....	33	system status.....	37
UK power cord.....	8	zoom waveform.....	45
USB driver installation.....	65	system status.....	37

勝特力材料 886-3-5753170
勝特力电子(上海) 86-21-34970699
勝特力电子(深圳) 86-755-83298787
[Http://www.100y.com.tw](http://www.100y.com.tw)